



## Correction to: Non-Uniform Microphone Arrays for Robust Speech Source Localization for Smartphone-Assisted Hearing Aid Devices

Anshuman Ganguly<sup>1</sup> · Issa Panahi<sup>1</sup>


Published online: 2 December 2017  
© Springer Science+Business Media, LLC, part of Springer Nature 2017

**Correction to: J Sign Process Syst (2017)**  
<https://doi.org/10.1007/s11265-017-1297-8>

In the original publication of the article, Fig. 1 was incorrect.  
The correct figure is shown below.

The authors regret the oversight.

**Figure 1** Signal Processing pipeline using Smartphone assisted HAD.

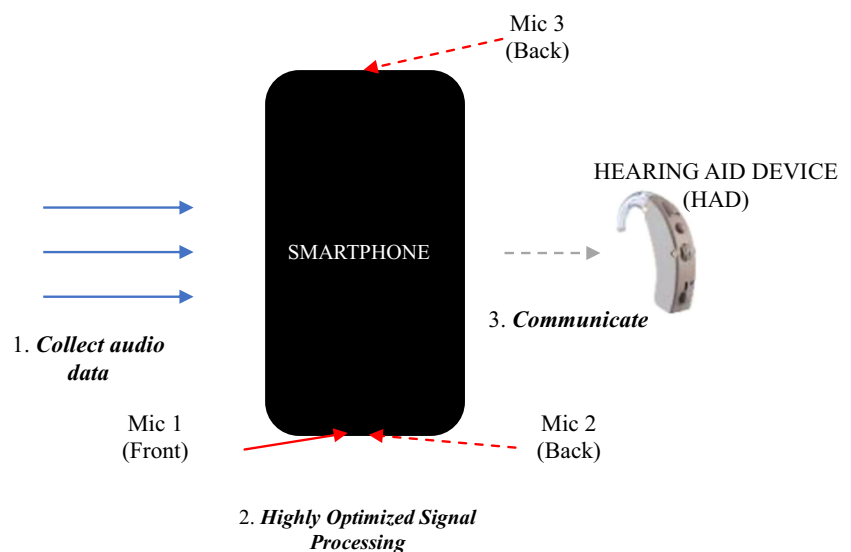

The online version of the original article can be found at <https://doi.org/10.1007/s11265-017-1297-8>.

✉ Anshuman Ganguly  
axg124330@utd.edu

Issa Panahi  
issa.panahi@utd.edu

<sup>1</sup> Department of Electrical Engineering, The University of Texas at Dallas, Richardson, TX 75080, USA