



Correction to: Retrieval analysis of contemporary antioxidant polyethylene: multiple material and design changes may decrease implant performance

Arianna Cerquiglini¹ · Johann Henckel¹ · Harry Hothi¹ · Lukas B. Moser^{2,3} · Antti Eskelin⁴ · Michael T. Hirschmann^{2,3} · Alister J. Hart¹

Published online: 31 August 2019
© European Society of Sports Traumatology, Knee Surgery, Arthroscopy (ESSKA) 2019

Correction to:
Knee Surgery, Sports Traumatology, Arthroscopy
(2019) 27:2111–2119
<https://doi.org/10.1007/s00167-019-05387-5>

Unfortunately, Fig. 1 caption was incorrectly updated in the original publication and correct Fig. 1 version is updated here.

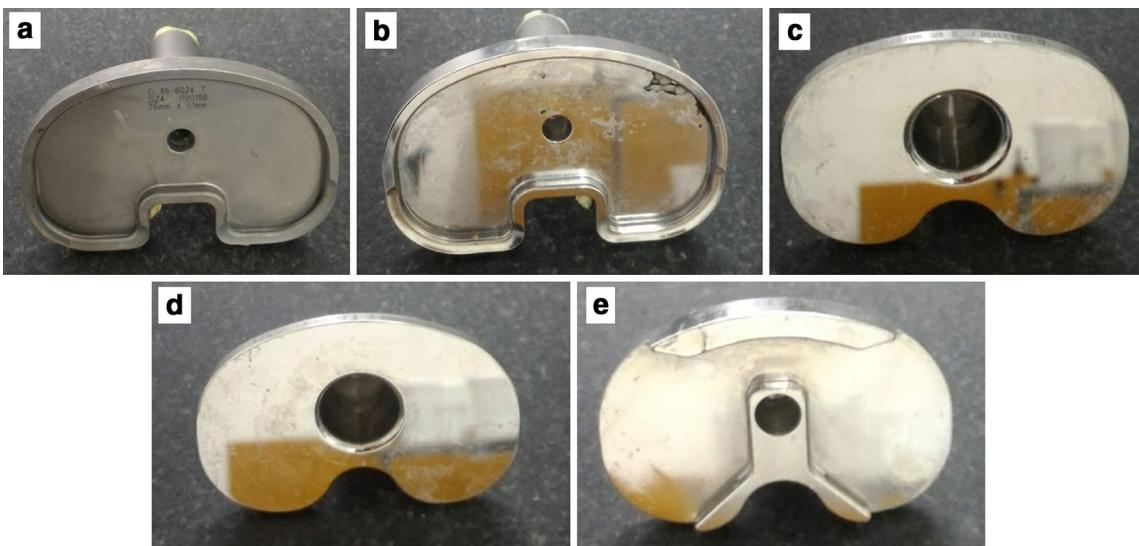


Fig. 1 Examples of two designs and relative iterations involved in the study: **a** Ti PFC fixed bearing, **b** CoCr PFC fixed bearing, **c** CoCr PFC RP, **d** Attune rotating bearing, **e** Attune fixed bearing

The original article can be found online at <https://doi.org/10.1007/s00167-019-05387-5>.

Publisher's Note Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.

✉ Arianna Cerquiglini
arianna.cerquiglini.15@ucl.ac.uk

¹ Institute of Orthopaedics and Musculoskeletal Science, University College London, Royal National Orthopaedic Hospital, Brockley Hill, Stanmore, Middlesex HA7 4LP, UK

² Department of Orthopaedic Surgery and Traumatology, Kantonsspital Basel (Bruderholz, Liestal, Laufen), Bruderholz, Switzerland

³ University of Basel, Basel, Switzerland

⁴ The Coxa Hospital for Joint Replacement, Tampere, Finland