


TECHNICAL DEVELOPMENTS



Ultra-low dose chest CT with silver filter and deep learning reconstruction significantly reduces radiation dose and retains quantitative information in the investigation and monitoring of lymphangiomyomatosis (LAM)

Alexa E. Golbus¹, Chloe Steveson², John L. Schuzer², Shirley F. Rollison³, Tat'Yana Worthy⁴, Amanda M. Jones⁵, Patricia Julien-Williams⁵, Joel Moss⁵ and Marcus Y. Chen^{1*} 

Abstract

Purpose Frequent CT scans to quantify lung involvement in cystic lung disease increases radiation exposure. Beam shaping energy filters can optimize imaging properties at lower radiation dosages. The aim of this study is to investigate whether use of SilverBeam filter and deep learning reconstruction algorithm allows for reduced radiation dose chest CT scanning in patients with lymphangiomyomatosis (LAM).

Material and methods In a single-center prospective study, 60 consecutive patients with LAM underwent chest CT at standard and ultra-low radiation doses. Standard dose scan was performed with standard copper filter and ultra-low dose scan was performed with SilverBeam filter. Scans were reconstructed using a soft tissue kernel with deep learning reconstruction (AiCE) technique and using a soft tissue kernel with hybrid iterative reconstruction (AIDR3D). Cyst scores were quantified by semi-automated software. Signal-to-noise ratio (SNR) was calculated for each reconstruction. Data were analyzed by linear correlation, paired *t*-test, and Bland–Altman plots.

Results Patients averaged 49.4 years and 100% were female with mean BMI 26.6 ± 6.1 kg/m². Cyst score measured by AiCE reconstruction with SilverBeam filter correlated well with that of AIDR3D reconstruction with standard filter, with a 1.5% difference, and allowed for an 85.5% median radiation dosage reduction (0.33 mSv vs. 2.27 mSv, respectively, $p < 0.001$). Compared to standard filter with AIDR3D, SNR for SilverBeam AiCE images was slightly lower (3.2 vs. 3.1, respectively, $p = 0.005$).

Conclusion SilverBeam filter with deep learning reconstruction reduces radiation dosage of chest CT, while maintaining accuracy of cyst quantification as well as image quality in cystic lung disease.

Clinical relevance statement Radiation dosage from chest CT can be significantly reduced without sacrificing image quality by using silver filter in combination with a deep learning reconstructive algorithm.

Key Points

- *Deep learning reconstruction in chest CT had no significant effect on cyst quantification when compared to conventional hybrid iterative reconstruction.*

*Correspondence:

Marcus Y. Chen
marcus.chen@nih.gov

Full list of author information is available at the end of the article




This is a U.S. Government work and not under copyright protection in the US; foreign copyright protection may apply 2024. **Open Access** This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>.

- SilverBeam filter reduced radiation dosage by 85.5% compared to standard dose chest CT.
- SilverBeam filter in coordination with deep learning reconstruction maintained image quality and diagnostic accuracy for cyst quantification when compared to standard dose CT with hybrid iterative reconstruction.

Keywords Deep learning, Radiation dosage, Tomography (X-ray computed), Lung diseases

Graphical abstract

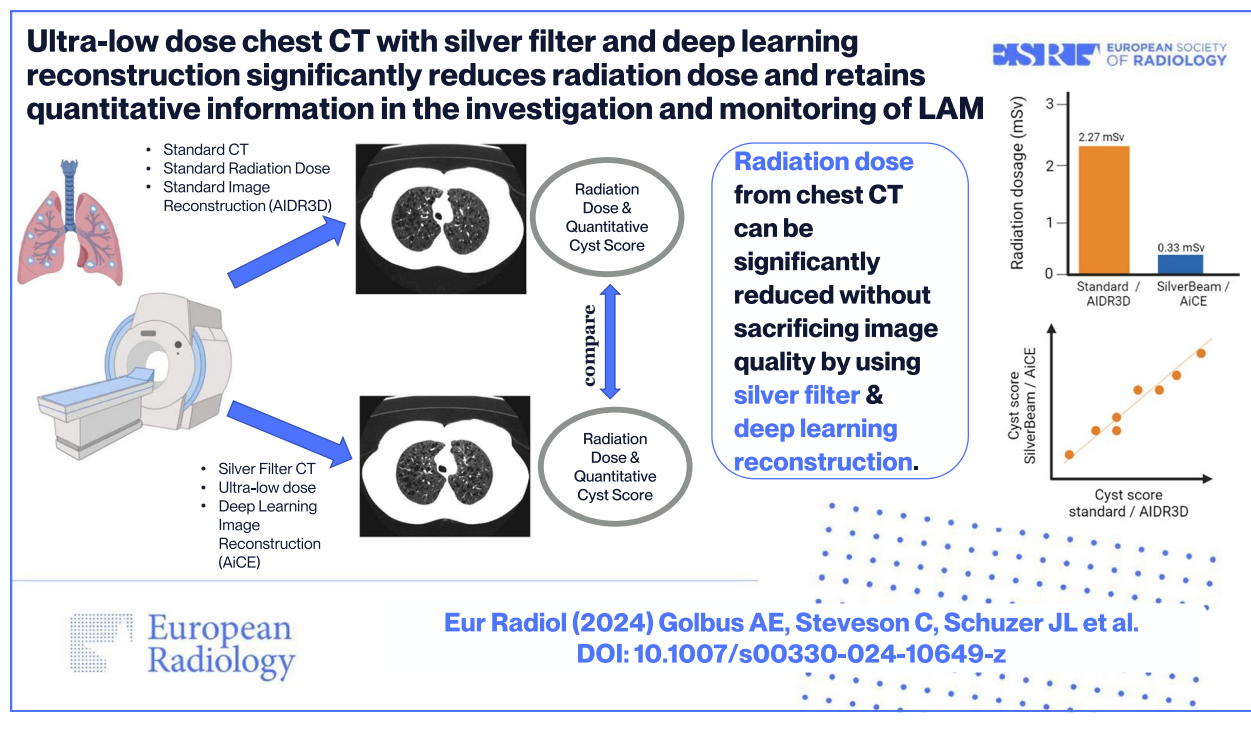

Introduction

Lymphangioleiomyomatosis (LAM) is a neoplastic disease, predominantly affecting women, and is characterized by infiltrative abnormal smooth muscle–like cells causing diffuse thin-walled pulmonary cysts [1]. While histologically benign, LAM cells express the lymphangiogenic growth factors VEGF-C and VEGF-D and spread through lymphatic channels [2]. Cystic destruction of the lungs leads to progressive deterioration of lung function [3]. The mTOR1 inhibitor sirolimus (rapamycin) is first-line treatment [4].

Quantification of lung involvement by CT scans can be performed [5]. The cyst score, defined as percentage of lung volume with lower attenuation and thus occupied by cysts, correlates to LAM disease severity as well as to physiologic data including pulmonary function testing and ventilation-perfusion scintigraphy [6, 7]. CT is superior to chest radiographs in evaluating extent of disease, particularly in identifying cysts <1.0 cm in diameter.

Disease progression and quantification of treatment response can be monitored by serial CT scans [7]. However, frequent CT scans increase radiation exposure. Ionizing radiation increases risk of hematologic and solid organ cancers [8–10]. Malignancy risk following exposure is increased in younger patients and in females [11, 12]. Therefore, methods to reduce radiation doses while maintaining accurate CT cyst score quantification is important in this population given need for regular CT scans.

Attempts to reduce CT radiation dosage have included the use of X-ray beam filtration. Tin and copper filters reduce radiation dosage without negatively impacting image quality, with copper filters now being the standard. However, silver filters have recently been studied for dose reduction [13, 14]. Although recent studies have assessed the impact of silver filter in combination with deep learning reconstruction on image quality and radiation doses in phantom chest models, this has not

been studied in clinical practice [8, 13, 15]. Image noise in ultra-low dose CT significantly degrades image quality when reconstructed with conventional methods; however, deep learning reconstruction can address this [16]. Deep learning reconstruction algorithms are known to improve image quality as assessed by signal-to-noise ratio (SNR) and contrast-to-noise ratio and have faster reconstruction speeds, compared to other reconstructions [8].

The aim of this study is to investigate whether the use of SilverBeam filter and a deep learning reconstruction algorithm allows for reduced radiation dose chest CT scanning.

Methods

With institutional review board approval (96-H-0100) and informed consent, 60 consecutive patients with lymphangiomyomatosis (LAM) were enrolled in this prospective study. Patients underwent chest CT at standard and ultra-low radiation doses on a 320-detector row CT scanner (Aquilion One Prism Edition, Canon Medical Systems) at a single center from November 2021 through August 2022. All CT scans were performed with 80×0.5 mm helical acquisition mode with 0.5 s gantry rotation time and standard pitch. For standard dose CT scans, X-ray tube potential and current were determined by automatic exposure control (SUREExposure 3D, Canon Medical), based on scout image attenuation, and used an image quality factor of SD12.5 and reconstructed using a soft tissue kernel with hybrid iterative reconstruction (Adaptive Iterative Dose Reduction (AIDR3D)). For standard filter images, a standard copper filter was used. Low-dose CT scans applied a SilverBeam filter and used fixed 120 kV and 80 mA and reconstructed using a soft tissue kernel with deep learning reconstruction (Advanced intelligent Clear-IQ Engine (AiCE)) techniques. Scanner-reported radiation dose parameters were documented based on the dose-length-product (DLP), for both the standard and low-dose scan protocols. The effective radiation dose in millisieverts (mSv) was calculated by multiplying dose-length-product by a conversion coefficient of 0.014 (mSv·mGy⁻¹·cm⁻¹) [17].

Images were reconstructed with 512×512 matrix, 2 mm slice thickness with 1 mm slice interval. Cyst scores (% of lung volume affected by cysts) were quantified by semi-automated software (Lung Density Analysis, Canon Medical) (Fig. 1). Signal-to-noise ratio (SNR) was calculated for each reconstruction. Data was analyzed by linear correlation, paired *t*-test, and Bland–Altman plots.

Results

Patients (*n*=60) averaged 49.4 years (range 23–70 years) and 100% were female with mean BMI 26.6±6.1 kg/m² (Table 1).

Ultra-low dose median radiation was reduced by 85.5% using SilverBeam filter with AiCE reconstruction compared to standard filter with AIDR3D reconstruction (0.33 (IQR 0.33–0.35) mSv vs. 2.27 (IQR 2.01–3.20) mSv, respectively, *p*<0.001) (Fig. 2). The median cyst score was 2.4 (IQR 0.4–13.4)% for SilverBeam filter with AiCE reconstruction versus 3.9 (IQR 1.0–14.3)% for standard filter with AIDR3D reconstruction, representing a difference of 1.5%. Linear correlation coefficient for cyst score quantified with imaging using SilverBeam filter with AiCE versus standard filter with AIDR3D was excellent at 0.98 (*p*<0.001) (Fig. 3a). Bland–Altman plot comparing difference in cyst score between the two showed a minimal negative bias of 1.23 (Fig. 3b). Linear correlation coefficient for cyst score of images reconstructed using AiCE compared to AIDR3D, with both using standard filter, was also excellent at 0.999 (*p*<0.001, Fig. 4a), with median cyst score of 3.7 (IQR 0.8–14.4)% vs. 3.9 (IQR 1.0–14.3)%, respectively (*p*<0.001). Bland–Altman plot showed minimal positive bias of 0.12 (Fig. 4b). Additionally, the linear correlation coefficient for cyst score quantified using SilverBeam filter with AIDR3D versus SilverBeam filter with AiCE was 0.98 (*p*<0.001), while the linear correlation coefficient for cyst score quantified with using SilverBeam filter with AIDR3D versus standard filter with AIDR3D was 0.92 (*p*<0.001).

Median signal-to-noise for imaging using SilverBeam filter with AiCE reconstruction was slightly lower than that of imaging using standard filter with AIDR3D reconstruction (3.1 (IQR 2.6–4.2) vs. 3.2 (IQR 2.7–4.7), respectively, *p*=0.005). Median SNR for standard filter with AiCE was significantly greater than that of standard filter with AIDR3D (3.9 (IQR 3.3–5.5) vs. 3.2 (IQR 2.7–4.7), respectively, *p*<0.001). SilverBeam filter with AiCE also had significantly greater SNR when compared to SilverBeam filter with AIDR3D (3.1 (IQR 2.6–4.2) vs. 1.9 (IQR 1.5–2.4), respectively, *p*<0.001).

Discussion

In our study, we evaluated the efficacy of SilverBeam filter with a deep learning reconstruction algorithm (AiCE) and found an 85.5% radiation dose reduction in chest CT scans of LAM patients. As pulmonary cysts in LAM are easily quantifiable, we utilized cyst score quantification as a metric to assess diagnostic accuracy of SilverBeam filter with AiCE. We compared the cyst score obtained using this filter and reconstruction to that quantified using the current traditional method and found that cyst score correlated strongly between images constructed using SilverBeam filter and AiCE reconstruction to those using standard filter and AIDR3D reconstruction, indicating that our method did not adversely impact diagnostic accuracy of cyst score quantification. Additionally,

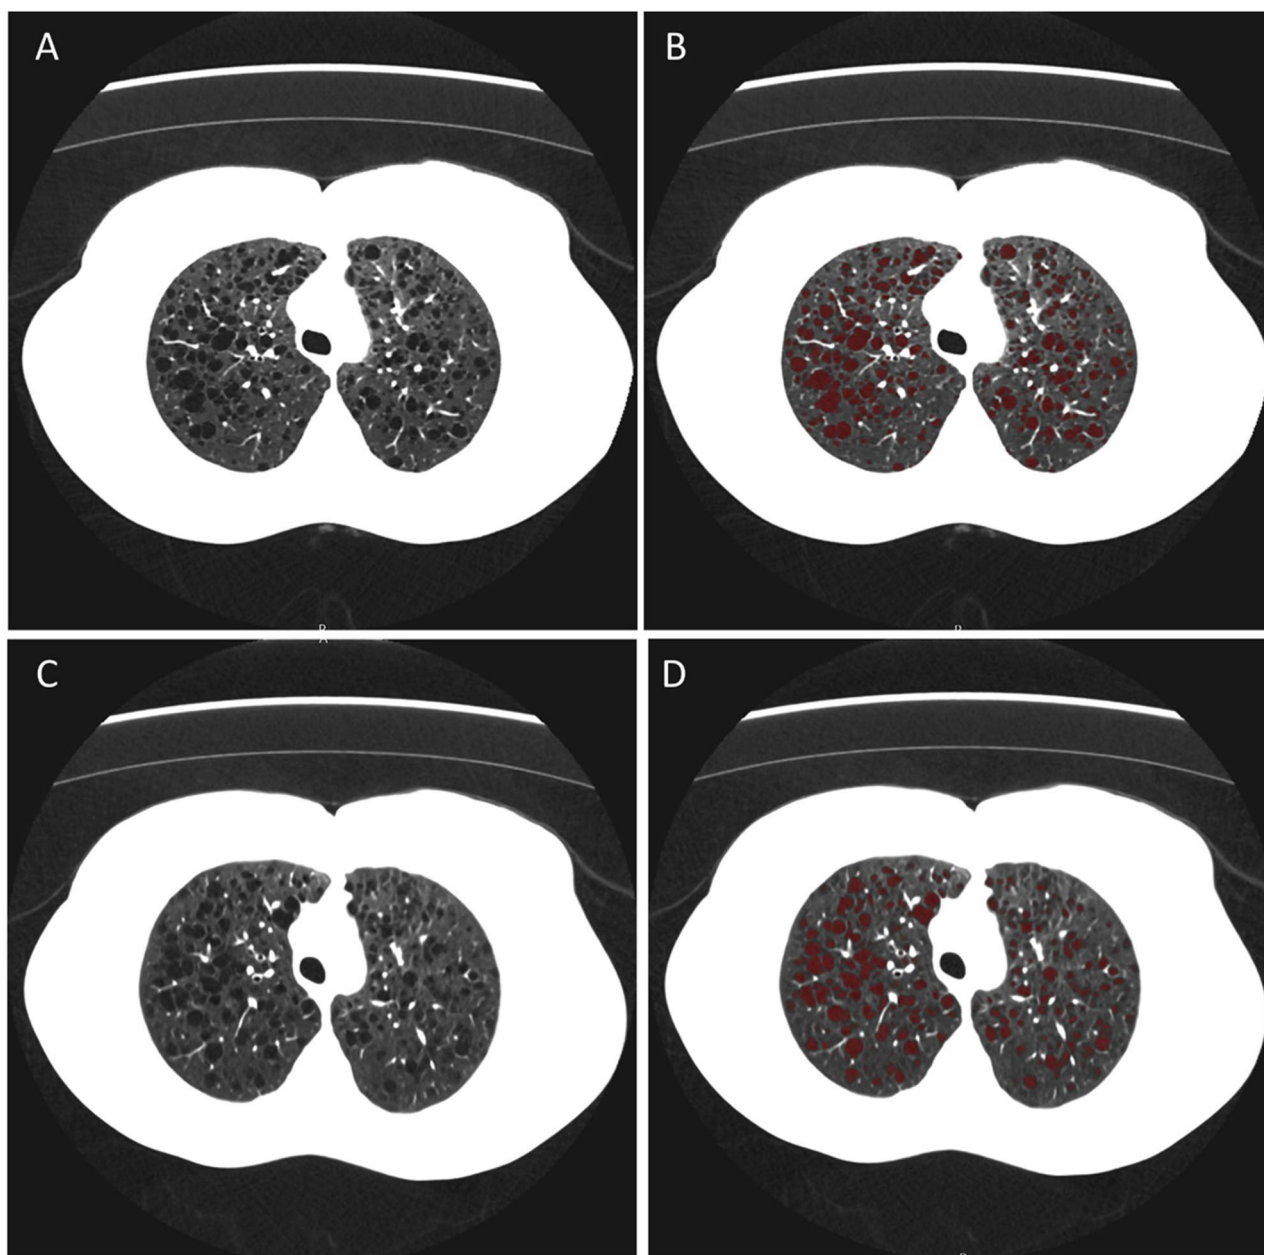


Fig. 1 Chest CT of a 29-year-old female with LAM. **A** Standard scan with ADR3D. **B** Standard scan with low attenuation areas highlighted in red. Radiation dose 1.90 mSv and cyst score 16.8%. **C** SilverBeam scan with AiCE. **D** SilverBeam scan with low attenuation areas highlighted in red. Radiation dose 0.33 mSv and cyst score 15.9%

we demonstrated that the reconstructive method (AiCE) itself did not alter diagnostic accuracy, as the cyst score obtained using standard filter with AiCE reconstruction correlated very strongly to that obtained using this same filter with ADR3D reconstruction. Nor did the SilverBeam filter itself negatively impact diagnostic accuracy, as there was a strong correlation in cyst score quantification between the SilverBeam filter and standard filter, with both using the same reconstructive method.

Although signal-to-noise ratio was slightly lower for imaging using SilverBeam filter with AiCE reconstruction compared to that using standard filter with ADR3D reconstruction, this difference of 0.1 is likely not large enough to be clinically significant. Comparing scans performed with the same filter but different reconstructions, AiCE allowed for a significantly greater SNR compared to ADR3D, and can be used in conjunction with SilverBeam filter to improve image quality. Our results

Table 1 Demographics of 60 patients with LAM

Sample size (n)	60
Gender (%F)	100%
Age (years) (mean ± standard deviation)	49.4 ± 12.4
Height (cm) (mean ± standard deviation)	164.2 ± 7.2
Weight (kg) (mean ± standard deviation)	71.8 ± 17.2
BMI (mean ± standard deviation)	26.6 ± 6.1
Ethnicity	75% non-Hispanic White 12% Asian 5% Black 5% Hispanic White 3% unknown

as a whole demonstrate that SilverBeam filter with AiCE reconstruction significantly reduces radiation dosage, while allowing for accurate cyst score quantification, without considerably affecting signal-to-noise ratio.

Although controversy exists surrounding the exact calculation of radiation risk, there have been recent advances in CT radiation dosage reduction [10], with one study showing that protocols including improved detector capability and tin filtration could reduce the risk of de novo lung cancer from lung cancer screening chest CT from 8.6 to 0.35 per 100,000 cases [10, 18]. In another study, standard dose chest CT (5 mSv) was shown to cause an increase in unstable chromosomal aberrations including DNA double strand breaks, whereas low-dose CT (classified as 1.5 mSv) did not [19]. In our study, SilverBeam filter reduced radiation to 0.33 mSv, which is below the threshold level of 1.5 mSv observed in this prior study. While radiation dose reduction in patients with LAM has previously been undertaken with ultra-low dose chest CT in combination with model based iterative reconstruction (MBIR), with a resulting 96% reduction in radiation (to a dosage of 0.14 mSv) [20], MBIR has lengthy computational times and image texture has

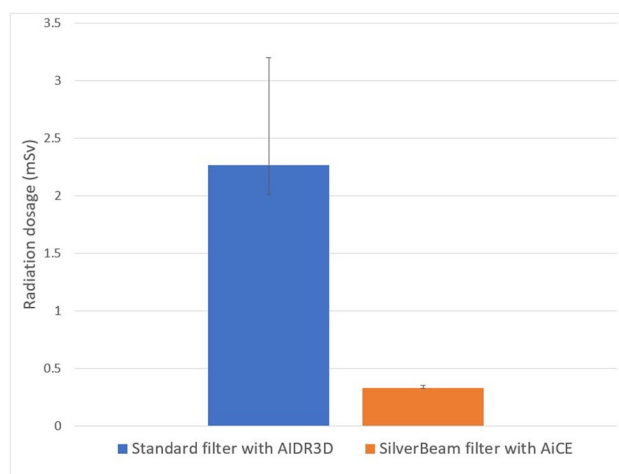


Fig. 2 Median effective radiation dosage (mSv) of standard filter with AIDR3D versus SilverBeam filter with AiCE was 2.27 (IQR 2.01–3.20) vs. 0.33 (IQR 0.33–0.35) mSv, respectively ($p < 0.001$), representing an 85.5% radiation dosage reduction

“plastic” or “artificial” appearance [8]. In our study, we were able to significantly reduce radiation dose, although not nearly to the extent of this prior study [20]; however, we were able to avoid sacrificing image quality by using deep learning image reconstruction (AiCE) rather than MBIR.

Silver X-ray beam spectral modification filters have recently been studied for radiation dose reduction [13–15]. Nomura et al. [14] evaluated the ability of a silver filter to reduce radiation of localizer radiography and found a 74% reduction in radiation dosage, compared to localizer radiographs using a copper filter. This study found that although detectability of anatomical landmarks was not negatively impacted, the image noise was significantly greater with silver filter compared to copper filter. While this study only evaluated radiation reduction of a silver filter in localizer imaging, we evaluated radiation reduction

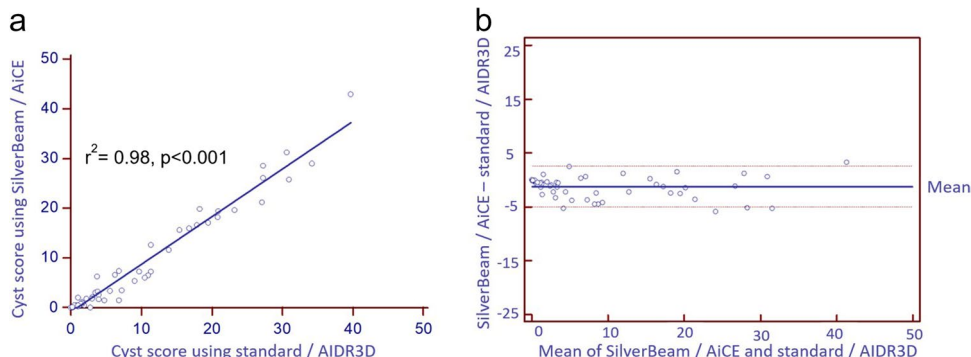


Fig. 3 a Linear regression of cyst score using SilverBeam filter with AiCE reconstruction versus standard filter with AIDR3D reconstruction. Median cyst score for SilverBeam with AiCE was 2.4 (IQR 0.4–13.4)% versus 3.9 (IQR 1.0–14.3)% for standard filter with AIDR3D, $r^2 = 0.98$, $p < 0.001$. **b** Bland–Altman plot showing mean negative bias of 1.23, with solid blue line indicating mean and red dashed lines indicating the bounds of the 95% confidence interval

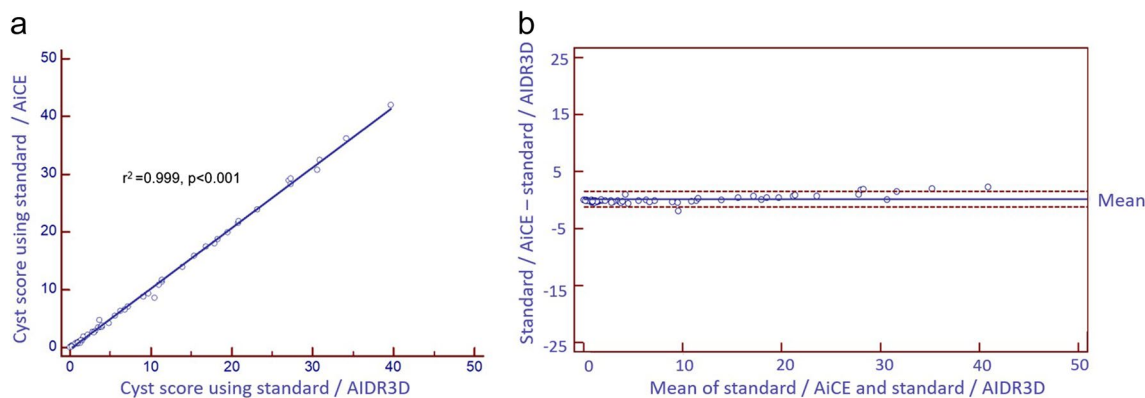


Fig. 4 **a** Linear regression of cyst score for AiCE vs. AIDR3D reconstruction using standard filter. Median cyst score 3.7 (IQR 0.8–14.4)% vs. 3.9 (IQR 1.0–14.3)%, respectively, $r^2 = 0.99$, $p < 0.001$. **b** Bland–Altman plot showing mean positive bias of 0.12 with solid blue line indicating mean and red dashed lines indicating the bounds of the 95% confidence interval

using a silver filter for the CT scan itself and found a similar percentage reduction in radiation. However, we additionally utilized deep learning (AiCE) reconstruction to preserve image quality and reduce noise despite the reduction in radiation dosage, and were largely able to maintain image quality as assessed by signal-to-noise ratio. Kawamoto et al. evaluated radiation dose characteristics and image quality when using silver filter with hybrid iterative reconstruction (AIDR3D) in phantom chests with a 10-mm nodule and found a reduction in image noise and artifacts when using a silver filter versus using no filter [15].

Recently, the ability of silver filter in combination with deep learning reconstruction, to detect lung nodules on phantom chests while reducing radiation dosage, was assessed [13]. Deep learning reconstruction (DLR) is a relatively new reconstructive method in CT that allows for preservation of image quality at lower radiation doses. While DLR has been evaluated in lung imaging including in nodule detection [21] and emphysema quantification [22], the combination of silver filters with DLR has only been evaluated in chest phantoms [13]. This study using phantom chests demonstrated that silver filter in combination with deep learning reconstruction reduces radiation dosage and increases median image quality score and nodule detection, compared to standard copper filter, with signal-to-noise ratio significantly greater for CT protocols using silver filter versus copper filter. We similarly found a reduction in radiation dosage using SilverBeam filter. However, we found SNR to be slightly lower with silver filter compared to standard copper filter. While this prior study had limitations specific to using phantom chests—particularly a lack of motion artifacts and no variability in body habitus that is present in clinical practice, as well as nodules that were perfectly round [13]—we demonstrated that

this reduction in radiation dosage is maintained in real patients in clinical practice when using SilverBeam filter with deep learning reconstruction. Therefore, while these prior studies using silver filter [13–15] had similar findings in terms of radiation reduction, our study was the first to assess radiation reduction using silver filter in combination with deep learning reconstruction, in CT scans of real patients.

While our study evaluated detection of pulmonary cysts in patients with LAM, a rare disease, the cyst score in LAM is evaluated by measuring percentage of low attenuation volume on CT. Similar methods to quantify the extent of airway and tissue involvement can assess disease severity in other emphysematous diseases such as COPD, and has been shown to correspond to histological measurements [16, 23, 24]. A deep learning convolutional neural network has been studied in combination with ultra-low dose CT in emphysema quantification indices [22]. Emphysema indices of ultra-low dose scans reconstructed with DLR did not significantly differ from that of standard-dose CT scans reconstructed with an adaptive statistical iterative reconstruction. Further, image noise was not different between the two, despite a reduction in radiation dosage from 3.43 mSv for standard dose scans to 0.39 mSv for ultra-low dose scans [22]. However, silver filter to reduce radiation dosage has not been evaluated in emphysema alone or otherwise in combination with a DLR algorithm.

Although our study is a single-center study, we expect this technique will yield similar results at other centers. The lower radiation dose scan utilized a fixed technique without attenuation-based tube current modulation and therefore, image quality and radiation dose savings are proportional to body size. While the cysts in LAM are homogenous, well delineated, and easily quantifiable, we expect that SilverBeam filter with deep learning reconstruction

in CT imaging in other diseases is likely to yield similar results in terms of radiation reduction with preservation of image quality and diagnostic accuracy. However, evaluation in other pulmonary diseases with less homogenous patterns is needed. Our findings suggest that SilverBeam filter in combination with deep learning reconstruction would likely be effective in reducing radiation dosage in imaging of other cystic or emphysematous diseases. Silver-Beam filter with DLR allows for a significant reduction in radiation while maintaining image quality and diagnostic accuracy in cystic lung disease.

Abbreviations

AiCE	Advanced intelligent Clear-IQ Engine
AIDR3D	Adaptive Iterative Dose Reduction
DLR	Deep learning reconstruction
LAM	Lymphangioliomyomatosis
SNR	Signal-to-noise ratio

Acknowledgements

We thank the LAM Foundation and the Tuberosus Sclerosis Alliance for their assistance in recruiting patients for our studies.

Funding

This work was supported by the Intramural Research Program, National Institutes of Health (NIH), National Heart, Lung, and Blood Institute (Bethesda, MD). This work was also made possible by the NIH Medical Research Scholars Program, a public-private partnership supported jointly by the NIH and contributions to the Foundation for the NIH from the American Association for Dental Research, the Colgate-Palmolive Company, and other private donors.

Declarations

Guarantor

The scientific guarantor of this publication is Marcus Chen.

Conflict of interest

The authors of this manuscript declare relationships with the following companies: NHLBI has an institutional research agreement (no funding) with Canon Medical Systems. Chloe Steveson and John Schuzer are employees of Canon Medical Systems.

Statistics and biometry

No complex statistical methods were necessary for this paper.

Informed consent

Written informed consent was obtained from all subjects (patients) in this study.

Ethical approval

Institutional Review Board approval was obtained (National Institutes of Health, 96-H-0100).

Study subjects or cohorts overlap

No study subjects or cohorts have been previously reported.

Methodology

- prospective
- experimental
- performed at one institution

Author details

¹Cardiovascular Branch, National Heart, Lung, and Blood Institute, National Institutes of Health, 10 Center Dr, MSC 1046, Building 10, Room B1D47, Bethesda, MD 20892, USA. ²Canon Medical Systems, Otawara, Japan. ³Radiology and Imaging Sciences, Clinical Center, National Institutes of Health, Bethesda, USA. ⁴Office of the Clinical Director, National Heart, Lung, and Blood Institute, National Institutes of Health, Bethesda, USA. ⁵Critical Care Medicine and Pulmonary Branch, National Heart, Lung, and Blood Institute, National Institutes of Health, Bethesda, USA.

Received: 16 November 2023 Revised: 19 December 2023 Accepted: 5 January 2024

Published online: 22 February 2024

References

- Xu KF, Xu W, Liu S et al (2020) Lymphangioliomyomatosis. *Semin Respir Crit Care Med* 41:256–268
- McCormack FX, Inoue Y, Moss J et al (2011) Efficacy and safety of sirolimus in lymphangioliomyomatosis. *N Engl J Med* 364:1595–1606
- Kundu N, Holz MK (2023) Lymphangioliomyomatosis: a metastatic lung disease. *Am J Physiol Cell Physiol* 324:320–326
- McCarthy C, Gupta N, Johnson SR, Yu JJ, McCormack FX (2021) Lymphangioliomyomatosis: pathogenesis, clinical features, diagnosis, and management. *Lancet Respir Med* 9:1313–1327
- Taveira-DaSilva AM, Moss J (2016) Epidemiology, pathogenesis, and diagnosis of lymphangioliomyomatosis. *Expert Opin Orphan Drugs* 4:369–378
- Taveira-DaSilva AM, Pacheco-Rodriguez G, Moss J (2010) The natural history of lymphangioliomyomatosis: markers of severity, rate of progression and prognosis. *Lymphat Res Biol* 8:9–19
- Gopalakrishnan V, Yao J, Steagall WK et al (2019) Use of CT imaging to quantify progression and response to treatment in lymphangioliomyomatosis. *Chest* 155:962–971
- McLeavy CM, Chunara MH, Gravell RJ et al (2021) The future of CT: deep learning reconstruction. *Clin Radiol* 76:407–415
- Tamm EP, Rong XJ, Cody DD, Ernst RD, Fitzgerald NE, Kundra V (2011) Quality initiatives: CT radiation dose reduction: how to implement change without sacrificing diagnostic quality. *Radiographics* 31:1823–1832
- May M, Heiss R, Koehnen J et al (2022) Personalized chest computed tomography: minimum diagnostic radiation dose levels for the detection of fibrosis, nodules, and pneumonia. *Invest Radiol* 57:148–156
- Law M, Ma WK, Lau D, Chan E, Yip L, Lam W (2016) Cumulative radiation exposure and associated cancer risk estimates for scoliosis patients: impact of repetitive full spine radiography. *Eur J Radiol* 85:625–628
- Ronckers CM, Land CE, Miller JS, Stovall M, Lonstein JE, Doody MM (2010) Cancer mortality among women frequently exposed to radiographic examinations for spinal disorders. *Radiat Res* 174:83–90
- Oshima Y, Ohno Y, Takenaka D et al (2023) Capability for dose reduction while maintaining nodule detection: comparison of silver and copper X-ray spectrum modulation filters for chest CT using a phantom study with different reconstruction methods. *Eur J Radiol* 166:110969
- Nomura K, Fujii K, Goto T et al (2021) Radiation dose reduction for computed tomography localizer radiography using an Ag additional filter. *J Comput Assist Tomogr* 45:84–92
- Kawamoto K, Sato H, Kogure Y (2023) Usefulness of Ag additional filter on image quality and radiation dose for low-dose chest computed tomography. *J Comput Assist Tomogr*. doi:10.1097/RCT.0000000000001538
- Mascalchi M, Camiciottoli G, Diciotti S (2017) Lung densitometry: why, how and when. *J Thorac Dis* 9:3319–3345
- McCullough C, Cody D, Edyvean S et al (2008) The measurement, reporting, and management of radiation dose in CT. *American Association of Physicists in Medicine, College Park*

18. Saltybaeva N, Martini K, Frauenfelder T, Alkadhi H (2016) Organ dose and attributable cancer risk in lung cancer screening with low-dose computed tomography. *PLoS One* 11:e0155722
19. Sakane H, Ishida M, Shi L et al (2020) Biological effects of low-dose chest CT on chromosomal DNA. *Radiology* 295:439–445
20. Hu-Wang E, Schuzer JL, Rollison S et al (2019) Chest CT scan at radiation dose of a posteroanterior and lateral chest radiograph series: a proof of principle in lymphangioleiomyomatosis. *Chest* 155:528–533
21. Jiang B, Li N, Shi X et al (2022) Deep learning reconstruction shows better lung nodule detection for ultra-low-dose chest CT. *Radiology* 303:202–212
22. Yeom JA, Kim KU, Hwang M et al (2022) Emphysema quantification using ultra-low-dose chest CT: efficacy of deep learning-based image reconstruction. *Medicina (Kaunas)* 58:939
23. Coxson HO, Leipsic J, Parraga G, Sin DD (2014) Using pulmonary imaging to move chronic obstructive pulmonary disease beyond FEV1. *Am J Respir Crit Care Med* 190:135–144
24. Jin H, Heo C, Kim JH (2019) Deep learning-enabled accurate normalization of reconstruction kernel effects on emphysema quantification in low-dose CT. *Phys Med Biol* 64:135010

Publisher's note

Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.