



Correction to: On-chip construction of a fully structured scaffold-free vascularized renal tubule

Yuntian Zhu¹ · Zhengdi Shi² · Weiping Ding² · Chengpan Li^{2,3}

Published online: 11 March 2023

© The Author(s), under exclusive licence to Springer Science+Business Media, LLC, part of Springer Nature 2023

Correction to: Biomed Microdevices

<https://doi.org/10.1007/s10544-023-00648-0>

The original version of this article unfortunately contained mistake. The background of Fig. 4 is incorrectly shown in black, making texts invisible. The correct image of Fig. 4 is the following.

The original article can be found online at <https://doi.org/10.1007/s10544-023-00648-0>.


✉ Weiping Ding
wpdings@ustc.edu.cn

✉ Chengpan Li
licp@ustc.edu.cn

¹ Hefei No. 1 High School, 230041 Hefei, Anhui, China

² School of Information Science and Technology, University of Science and Technology of China, Hefei, Anhui 230027, China

³ Center for Biomedical Imaging, University of Science and Technology of China, Hefei, Anhui 230027, China

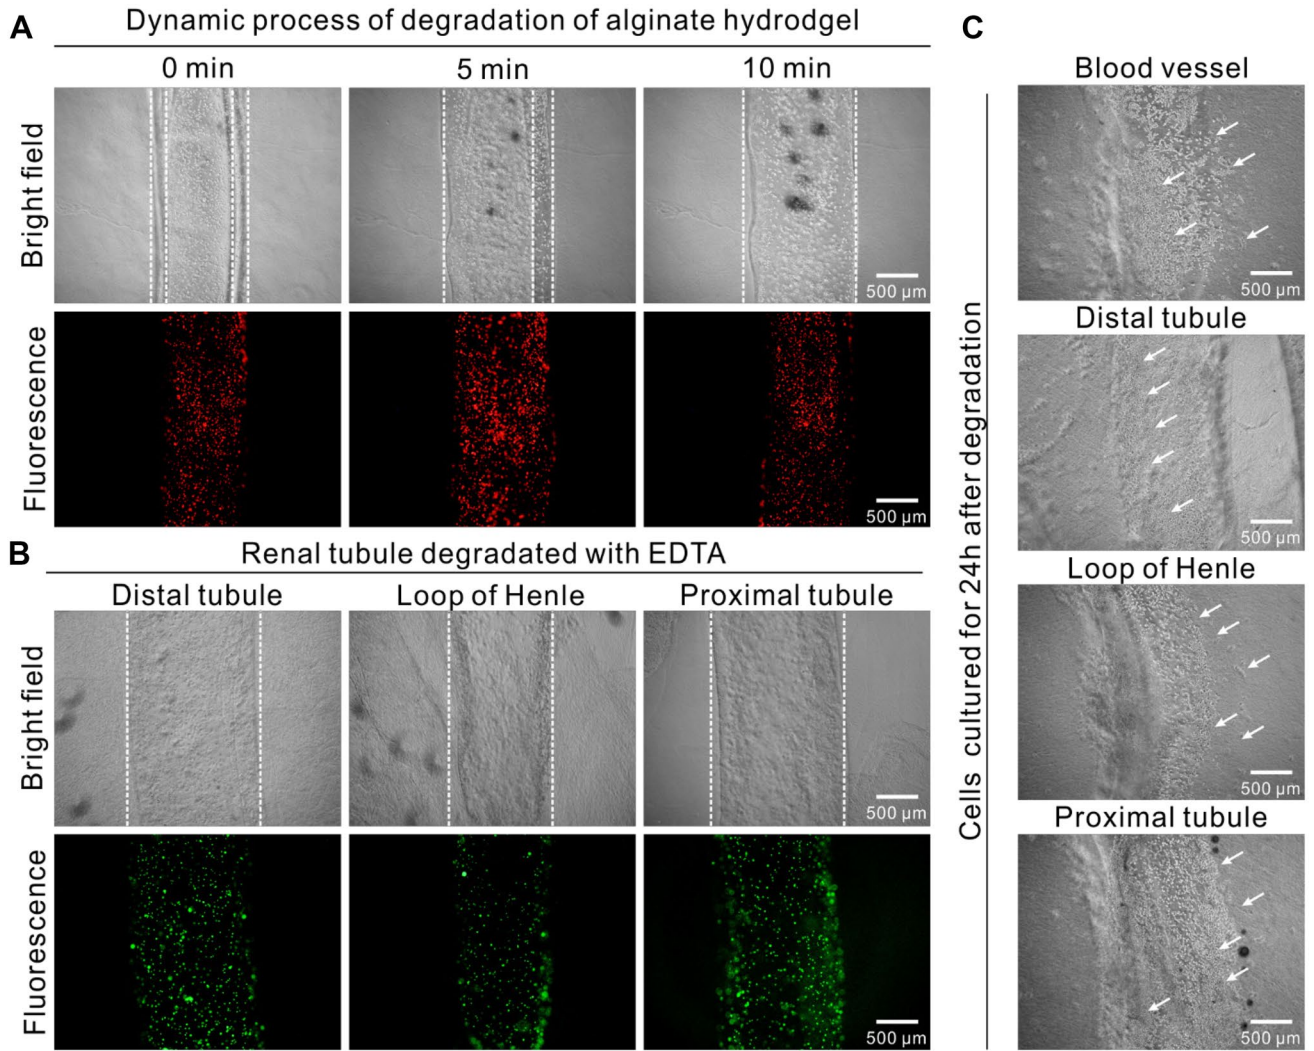

The original article has been corrected.

Publisher's Note Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.