


## ARTICLE



# Influence of decentration and tilt of Tecnis ZCB00 on visual acuity and higher order aberrations

Elena Martínez-Plaza<sup>1,2</sup>, Alberto López-de la Rosa<sup>1</sup>, Eleni Papadatou<sup>3</sup>, Nabil E. Habib<sup>4</sup>, Antonio J. Del Águila-Carrasco<sup>3</sup>, Alberto López-Miguel<sup>1,2</sup>✉, Miguel J. Maldonado<sup>1,2</sup> and Phillip J. Buckhurst<sup>3</sup> 

© The Author(s), under exclusive licence to The Royal College of Ophthalmologists 2022

**BACKGROUND/OBJECTIVES:** To determine the influence of decentration and tilt of a pseudophakic aspheric intraocular lens (IOL) on visual acuity (VA) and higher-order aberrations (HOAs), and to analyze the agreement between pupil center/axis and iridocorneal angles center/axis when assessing IOL decentration and tilt.

**SUBJECTS/METHODS:** A prospective interventional case series study including thirty-three patients undergoing Tecnis ZCB00 (Abbott Medical Optics) implantation. IOL decentration and tilt with respect to two reference systems (pupil and iridocorneal angles centers/axes), in cartesian (X,Y) and polar (radius/tilt, polar angle/azimuth) coordinates, were assessed with optical coherence tomography. VA and internal and ocular HOAs were evaluated. Multiple linear regression models and intraclass correlation coefficient (ICC) were computed.

**RESULTS:** IOL decentration only showed a significant effect on internal HOAs for  $Z_3^3$  ( $R^2 = 0.20$ ,  $P = 0.04$ ). IOL decentration with respect to the pupil center showed a significant effect on ocular  $Z_3^{-3}$  ( $R^2 = 0.18$ ,  $P = 0.05$ ),  $Z_3^1$  ( $R^2 = 0.36$ ,  $P = 0.001$ ) and  $Z_4^{-4}$  ( $R^2 = 0.24$ ,  $P = 0.02$ ); and with respect to the center of iridocorneal angles, on ocular  $Z_3^3$  ( $R^2 = 0.21$ ,  $P = 0.03$ ),  $Z_4^2$  ( $R^2 = 0.32$ ,  $P = 0.003$ ), primary coma ( $R^2 = 0.41$ ,  $P < 0.001$ ), and coma-like ( $R^2 = 0.40$ ,  $P = 0.001$ ). Poor agreement between both reference systems was found for IOL decentration measurements ( $ICC \leq 0.41$ ), except for the polar angle coordinate ( $ICC = 0.83$ ). Tilt measurements showed good agreement ( $ICC \geq 0.75$ ).

**CONCLUSIONS:** Tecnis ZCB00 decentration and tilt values after uneventful implantation appear not to have influence on VA, and their effect on HOAs are not high enough to clinically affect quality of vision. Pupil and iridocorneal angles used as reference systems may be interchangeable for IOL tilt measurements, but not for decentration.

Eye (2023) 37:1640–1645; <https://doi.org/10.1038/s41433-022-02211-2>

## INTRODUCTION

The positive primary spherical aberration (SA) of the cornea is usually compensated by the negative SA of the crystalline lens in the youthful eye. Morphological changes experienced by the lens with age (e.g., thickness and opacification) can result in less negative or even positive SA, degrading the optical quality of the eye [1–3]. Crystalline lens opacification is the leading cause of ophthalmological surgery worldwide, with phacoemulsification and pseudophakic intraocular lens (IOL) implantation being the standard procedures used in cataract surgery within developed countries [4].

Several optical designs for pseudophakic IOLs have been developed which vary in the amount of SA induced. Spherical IOL designs add positive SA [5], in contrast, aspheric IOL designs either; avoid the induction of SA (aberration-free IOLs), partially compensate the SA of the cornea (i.e., SA of  $-0.20 \mu\text{m}$ ) [6], or fully compensate the SA of the cornea (SA of approximately  $-0.27 \mu\text{m}$ ) [7–9]. Numerous authors have reported that aspheric IOLs provide better photopic and mesopic contrast sensitivity in comparison to spherical IOLs [10–14]. However, decentration and tilt of

aspheric IOLs have a greater impact on optical quality than spherical ones [15].


Decentration and tilt are one of the most frequent complications that can be present even after uneventful IOL implantation [16]. Numerous theoretical and experimental works have analyzed the influence of decentration and tilt of aspheric IOLs on optical quality using model eyes or simulators [17–19]. Nonetheless, in-vivo clinical studies continue to be of great interest to properly understand the effect of aspheric IOL decentration and tilt on visual performance. In addition, there is not a gold standard method to assess decentration and tilt. Previous studies have used different methods such as Purkinje images, Scheimpflug images or Optical Coherence Tomography, with no universal reference points and axes [20].

The aim of the present study was to determine the influence of decentration and tilt on visual acuity (VA) and higher-order aberrations (HOAs) after the implantation of an aspheric IOL with negative SA (Tecnis® ZCB00, Abbott Medical Optics; Santa Ana, CA). Additionally, the agreement between pupil center and axis and iridocorneal angles center and axis to assess decentration and tilt was also evaluated.

<sup>1</sup>Instituto de Oftalmobiología Aplicada (IOBA), Universidad de Valladolid, Valladolid, Spain. <sup>2</sup>Red Temática de Investigación Colaborativa en Oftalmología (OftaRed), Instituto de Salud Carlos III, Madrid, Spain. <sup>3</sup>Faculty of Health, University of Plymouth, Plymouth, UK. <sup>4</sup>Royal Eye Infirmary, University Hospitals Plymouth NHS Trust, Plymouth, UK. ✉email: [alopezm@ioba.med.uva.es](mailto:alopezm@ioba.med.uva.es)

Received: 17 December 2021 Revised: 23 June 2022 Accepted: 10 August 2022

Published online: 24 August 2022

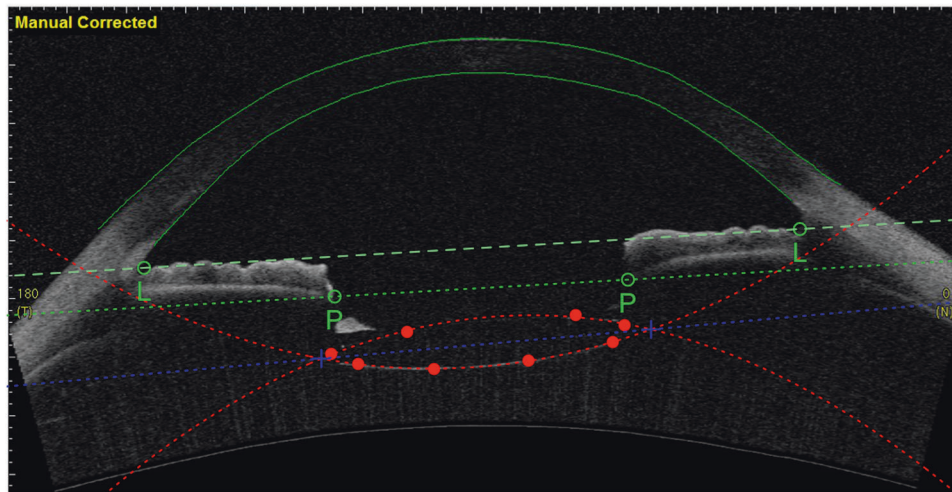

**Fig. 1 Segmentation of the swept-source optical coherence tomography image showing an implanted Tecnis® ZCB00.** Manual segmentation of the cornea (continuous tracing) is shown. Coordinates and line between iridocorneal angles (L, dashed lines tracing), coordinates and line between inner edges of the iris (P, tracing with circle symbols), intraocular lens surfaces (tracing with filled circle symbols) and intraocular lens tilt (tracing with plus symbols).

## METHODS

The present work is a prospective case series study. It was approved by the United Kingdom National Health Service (NHS) and the University of Plymouth faculty of Health Research ethics committee. Procedures were performed in accordance with the Declaration of Helsinki and all participants provided written informed consent.

### Intraocular lens specifications

Tecnis ZCB00 is a biconvex one-piece monofocal IOL with an anterior prolate surface (aspheric design) inducing a negative SA of  $-0.27 \mu\text{m}$ . This lens is made by hydrophobic acrylic material with a continuous  $360^\circ$  posterior square edge design and offset haptics. IOL presents a 6.0 mm optical diameter with a range correction from  $+5.0$  diopters (D) to  $+34.0$  D.

### Sample

Thirty-three eyes of 33 volunteers who underwent Tecnis ZCB00 implantation in at least one eye were assessed. Inclusion criteria were patients aging 18 years or older, and uneventful phacoemulsification with IOL implantation surgery performed 3–12 months prior to the examination visit. Exclusion criteria were patients with amblyopia, glaucoma, retinal or corneal diseases, iris and pupil anomalies or any previous ocular surgery.

In cases where patients underwent Tecnis ZCB00 implantation in both eyes, the study eye selected was the first implanted one. The contralateral eye was occluded during eye examinations.

### Study parameters

Monocular uncorrected distance visual acuity (UDVA) was assessed using a computerized test chart (POLA VistaVision - DMD Med Tech, Italy) at 6 m distance. The logarithm of the minimum angle of resolution (logMAR) was recorded for each patient.

Internal and ocular aberrations were obtained with the OPD-Scan III system (Nidek Technologies, Japan). The following second-order Zernike coefficients and higher-order aberrations (HOAs) for a 4 mm pupil diameter were selected for study purposes: second-order Zernike coefficients ( $Z_2^{-2}$ ,  $Z_2^0$  and  $Z_2^2$ ), third and four-order Zernike coefficients ( $Z_3^{-3}$ ,  $Z_3^{-1}$ ,  $Z_3^1$ ,  $Z_3^3$ ,  $Z_4^{-4}$ ,  $Z_4^{-2}$ ,  $Z_4^0$ ,  $Z_4^2$  and  $Z_4^4$ ), secondary spherical aberration ( $Z_0^0$ ), primary ( $Z_3^{-1}$  and  $Z_3^1$ ) and secondary ( $Z_5^{-1}$  and  $Z_5^1$ ) coma root mean square (RMS), coma-like ( $Z_3^{-1}$ ,  $Z_3^1$ ,  $Z_5^{-1}$  and  $Z_5^1$ ) RMS, spherical-like ( $Z_4^0$  and  $Z_6^0$ ) RMS, and total HOAs RMS (from 3rd to 6th order). Keratometry and asphericity data were also obtained from OPD-Scan III system. Axial length measurements were performed preoperatively using the IOLMaster 500 (Zeiss, Jena, Germany).

### Assessment of intraocular lens tilt and decentration

A swept-source optical coherence tomography (ss-OCT) system (Casia SS-1000, Tomey, Japan) was used to obtain anterior segment images selecting the radial 3-D angle analysis. The measurements were performed under

mydriasis after instilling one drop of Phenylephrine 2.5% (Minims Phenylephrine Hydrochloride®; Bausch & Lomb, United Kingdom) and Tropicamide 1.0% (Minims Tropicamide®; Bausch & Lomb, United Kingdom), respectively.

Firstly, 12 sectional images, corresponded to the following meridians: 0–180, 15–195, 30–210, 45–225, 60–240, 75–255, 90–270, 105–285, 120–300, 135–315, 150–330 and 165–345 degrees were selected. The anatomical structures of the anterior segment of the eye (including the IOL) were properly identified using the manual tool of the ss-OCT software and the RStudio software (1.0.143 version) (Fig. 1). Thus, the distance between the center of each reference system (pupil center or iridocorneal angles) and the center of the IOL was measured for each image. In addition, the angular distance between each reference system axis and the IOL axis was also determined for each image. This measurement procedure was performed in the 12 selected images per subject.

To measure the IOL decentration parameters, the 12 images were grouped into perpendicular pairs (A: 0–180 and 90–270 degrees, B: 15–195 and 105–285 degrees, C: 30–210 and 120–300 degrees, D: 45–225 and 135–315 degrees, E: 60–240 and 150–330 degrees, and F: 75–255 and 165–345 degrees) creating six individual reference systems, each rotated  $15^\circ$  from the anterior one (Supplementary Fig. S1). Distance values between each reference system (pupil center or iridocorneal angles) and IOL previously calculated in the 12 sections, were considered as  $x'$  or  $y'$  coordinates (Supplementary Fig. S1). The resultant distance and the resultant angle of each individual reference coordinates system (From A to F) were calculated. Finally, the mean values of the six systems were also calculated. The IOL decentration was determined using cartesian (X, Y) and polar coordinates (radius and polar angle). Regardless of the eye evaluated, positive values of the X-coordinate indicated nasal decentrations, while negative values indicated temporal decentrations. Regarding the Y-coordinate, positive values meant superior decentrations.

Tilt was defined as the angle between the reference plane (pupil axis and iridocorneal angles axis) and the IOL plane. Azimuth was defined as the IOL tilt orientation (angle of the IOL tilt normal vector projected on the reference plane). Similar to the IOL decentration assessment performed, IOL tilt was measured using the 12 images grouped into perpendicular pairs (From A to F) to calculate cartesian (X, Y) and polar coordinates (tilt and azimuth). The geometrical method developed to calculate IOL tilt and azimuth is provided in the Supplementary Information (Supplementary Fig. S2). Regardless of the eye evaluated, positive values of IOL tilt in the X-coordinate indicated nasal azimuths, while negative values indicated temporal azimuths.

### Statistical analysis

The statistical analysis was performed using R statistical package version 4.0.0 (The R Foundation, Vienna, Austria). Sample size was estimated taking into account that two independent variables were considered in each regression model, establishing a large effect size ( $f^2$ ) of 0.35 [21] and

**Table 1.** Mean values of internal and ocular aberrations.

HOAs	Internal ( $\mu\text{m}$ ) Mean $\pm$ SD	Ocular ( $\mu\text{m}$ ) Mean $\pm$ SD
$Z_2^{-2}$	0.006 $\pm$ 0.124	0.002 $\pm$ 0.153
$Z_2^0$	0.109 $\pm$ 0.757	0.228 $\pm$ 0.238
$Z_2^2$	0.185 $\pm$ 0.376	0.142 $\pm$ 0.319
$Z_3^{-3}$	-0.036 $\pm$ 0.182	-0.047 $\pm$ 0.143
$Z_3^{-1}$	0.019 $\pm$ 0.143	-0.046 $\pm$ 0.533
$Z_3^1$	0.011 $\pm$ 0.058	-0.009 $\pm$ 0.054
$Z_3^3$	0.002 $\pm$ 0.080	0.001 $\pm$ 0.099
$Z_4^{-4}$	0.009 $\pm$ 0.053	-0.015 $\pm$ 0.036
$Z_4^{-2}$	0.009 $\pm$ 0.037	0.001 $\pm$ 0.025
$Z_4^0$	-0.064 $\pm$ 0.086	-0.018 $\pm$ 0.024
$Z_4^2$	-0.009 $\pm$ 0.078	-0.004 $\pm$ 0.037
$Z_4^4$	-0.015 $\pm$ 0.080	-0.019 $\pm$ 0.037
Primary coma (RMS)	0.091 $\pm$ 0.125	0.075 $\pm$ 0.048
Secondary coma (RMS)	0.033 $\pm$ 0.055	0.014 $\pm$ 0.008
Coma-like (RMS)	0.098 $\pm$ 0.136	0.077 $\pm$ 0.475
$Z_6^0$	0.010 $\pm$ 0.032	0.002 $\pm$ 0.005
Spherical-like (RMS)	0.089 $\pm$ 0.069	0.026 $\pm$ 0.015
Total (RMS)	0.240 $\pm$ 0.215	0.203 $\pm$ 0.084

RMS root mean square, SD standard deviation.

assuming a two-sided level of significance of 0.05 and a statistical power of 80%. The minimum sample size needed was 31 patients.

The agreement between IOL decentration and tilt values for both reference systems, pupil center/axis and center/axis of the line joining iridocorneal angles, was analyzed by the absolute agreement intraclass correlation coefficient (ICC) [22]. To analyze the angular differences in polar angle and azimuth parameters, when angular differences between reference systems exceeded 180 degrees, coterminal angles were calculated for pupil center/axis reference system.

The effect of age and IOL power on the decentration and tilt parameters was analyzed by using simple linear regressions. The assumptions of normality, homoscedasticity, linearity and lack of outliers were checked using the residuals of the fitted models.

The effect of the IOL decentration on the study parameters was analyzed by fitting two multiple linear regression models per each study variable, including the cartesian (X, Y) or polar coordinates (radius, polar angle), for each reference system. Similarly, two multiple linear regression models per variable were used to analyze the effect of tilt coordinates (X, Y) or total tilt coordinates (tilt and azimuth), for each reference system. The required model assumptions (normality, homoscedasticity, linearity and lack of outliers) were checked. Two-sided P-values  $\leq$  0.05 were considered statistically significant.

## RESULTS

### Study population

A total of 33 (23 females and 10 males) patients with a mean age of  $72.9 \pm 6.9$  years were included. The mean axial length was  $23.49 \pm 1.32$  mm. The mean IOL power was  $21.98 \pm 4.35$  D. The mean UDVA and the mean spherical equivalent was  $0.13 \pm 0.13$  logMAR and  $-0.48 \pm 0.40$  D, respectively. The mean flat and steep keratometry was  $43.03 \pm 1.86$  D and  $44.26 \pm 1.78$  D, respectively. The mean corneal asphericity was  $-0.15 \pm 0.26$ . Table 1 shows the mean HOAs values.

### Decentration and tilt

The mean horizontal decentration of the IOL was nasal according to both the pupil center ( $0.04 \pm 0.17$  mm) and iridocorneal angles ( $0.18 \pm 0.16$  mm). For vertical decentration, on average, a superior

location was observed (pupil center,  $0.17 \pm 0.19$  mm; iridocorneal angles  $0.06 \pm 0.26$  mm. Table 2; Fig. 2A).

Absolute tilt was similar according to both the pupil axis ( $2.52 \pm 1.21$  degrees) and axis of the line joining iridocorneal angles ( $2.64 \pm 1.09$  degrees) (Table 2; Fig. 2B).

The agreement between decentration and tilt for both reference systems is shown in Table 2.

No effect of age on decentration and tilt was found ( $P \geq 0.16$ ). However, a significant relationship was found between IOL power and Y-coordinate with respect to the pupil center ( $\beta = 0.02$ , 95% confidence interval (CI): 0.00/0.04;  $P = 0.02$ ), and between IOL power and X-coordinate with respect to the center of iridocorneal angles ( $\beta = 0.01$ , 95% CI: 0.00/0.03;  $P = 0.04$ ).

### Effect of IOL decentration and tilt on visual acuity and aberrations

Neither IOL decentration or tilt had a significant influence on UDVA ( $P \geq 0.13$ ) or second-order Zernike coefficients ( $P \geq 0.06$ ).

IOL decentration, as measured with cartesian coordinates, with respect to the center of the line joining iridocorneal angles showed a significant influence on the internal  $Z_3^3$  ( $R^2 = 0.20$ ,  $P = 0.04$ ), specifically, the X-coordinate ( $\beta = -0.19$ ; 95% CI:  $-0.35/-0.02$ ;  $P = 0.03$ ). No significant ( $P \geq 0.14$ ) effect of IOL decentration with respect to the pupil center system was found on internal HOAs. Similarly, IOL tilt did not have a significant ( $P \geq 0.09$ ) effect on any internal HOA with respect to any reference system.

IOL decentration, as measured with cartesian coordinates, in relation to the pupil center showed a significant effect on ocular  $Z_3^{-3}$  ( $R^2 = 0.18$ ,  $P = 0.05$ ),  $Z_3^1$  ( $R^2 = 0.36$ ,  $P = 0.001$ ) and  $Z_4^{-4}$  ( $R^2 = 0.24$ ,  $P = 0.02$ ). In addition, IOL decentration, as measured with cartesian coordinates, with respect to the center of iridocorneal angles had a significant effect on the following ocular HOAs:  $Z_3^3$  ( $R^2 = 0.21$ ,  $P = 0.03$ ),  $Z_4^2$  ( $R^2 = 0.32$ ,  $P = 0.003$ ), primary coma ( $R^2 = 0.41$ ,  $P < 0.001$ ), and coma-like ( $R^2 = 0.40$ ,  $P = 0.001$ ). Likewise, when IOL decentration was described in terms of polar coordinates, it showed a significant effect on ocular  $Z_4^2$  ( $R^2 = 0.26$ ,  $P = 0.02$ ). Table 3 shows the coordinates with a significant effect on ocular HOAs. Regarding ocular  $Z_3^{-3}$ , the linear regression model showed a significant effect on this HOA, however, each individual coordinate (X,Y) respect to the pupil did not show any significant ( $P \geq 0.06$ ) effect on ocular  $Z_3^{-3}$ . Besides, IOL tilt did not have a significant effect on any ocular HOA with respect to any reference system ( $P \geq 0.06$ ).

## DISCUSSION


The present study showed the Tecnis ZCB00 decentration and tilt after uneventful cataract surgeries using two reference systems (pupil center (or axis) and center (or axis) of iridocorneal angles), and analyzed its effect on VA and HOAs. Decentration and tilt of the Tecnis ZCB00 as measured with a new method based on ss-OCT images, did not have a significant effect on VA, but had an influence on some ocular HOAs and internal  $Z_3^3$  aberration. Additionally, the agreement between both reference systems in cartesian and polar coordinates was also evaluated. It was observed that decentration values are not interchangeable except for polar angle, whilst the tilt reference angles showed high agreement.

To our knowledge, there is not a gold standard method for measuring IOL decentration and tilt [20], thus, the present study assessed the agreement between two reference systems: pupil center/axis and iridocorneal angles center/axis. The agreement found for decentration measurements was poor (ICC  $\leq$  0.41) except for the polar angle coordinate, which presented good agreement (ICC = 0.83). The lack of agreement is likely a consequence of a discrepancy between the location of the pupil center and the center of the iridocorneal angles [23]. However, tilt measurements in cartesian and polar coordinates with respect to the pupil and

**Table 2.** Mean and agreement of decentration and tilt values measured with respect to the pupil center (or axis) or center (or axis) of the line joining iridocorneal angles.

		Pupil center/axis (mean $\pm$ SD)	Iridocorneal angles center/axis (mean $\pm$ SD)	Agreement ICC (CI 95%)	P-value
Decentration	X-coordinate (mm)	0.04 $\pm$ 0.17	0.18 $\pm$ 0.16	0.41 (–0.01/0.69)	0.038
	Y-coordinate (mm)	0.17 $\pm$ 0.19	0.06 $\pm$ 0.26	0.28 (–0.04/0.55)	0.041
	Radius (mm)	0.28 $\pm$ 0.11	0.34 $\pm$ 0.10	0.37 (0.05/0.62)	0.012
	Polar angle (degrees)	181.19 $\pm$ 160.66	155.96 $\pm$ 131.35	0.83 (0.68/0.91)	<0.001
Tilt	X-tilt (degrees)	0.58 $\pm$ 1.81	0.76 $\pm$ 1.84	0.85 (0.72/0.92)	<0.001
	Y-tilt (degrees)	–0.75 $\pm$ 1.95	0.01 $\pm$ 2.10	0.75 (0.46/0.88)	<0.001
	Tilt (degrees)	2.52 $\pm$ 1.21	2.64 $\pm$ 1.09	0.83 (0.68/0.91)	<0.001
	Azimuth (degrees)	197.47 $\pm$ 134.29	202.41 $\pm$ 122.23	0.92 (0.85/0.96)	<0.001

CI coefficient interval, ICC intraclass correlation coefficient, SD standard deviation.

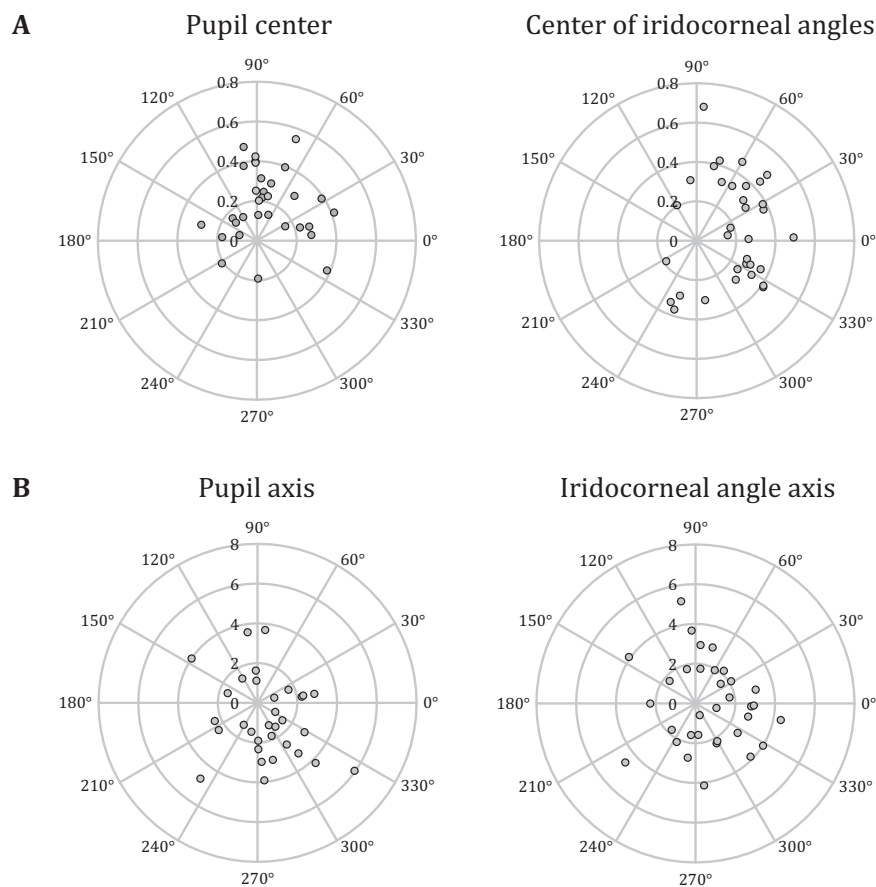

**Fig. 2** Polar plots of the decentration and tilt of the Tecnis® ZCB00 in relation to the pupil center or axis, and center or axis of iridocorneal angles. In the decentration plots (A), the radius (mm) and polar angle (degrees) are shown as the distance from the center of the axis (0.2 mm per ring) and the orientation, respectively. In the tilt plots (B), tilt (degrees) and azimuth (degrees) are shown as the distance from the center of the axis (2 degrees per ring) and the orientation, respectively. (0°: nasal; 180°: temporal).

iridocorneal angles axes showed good ( $ICC \geq 0.75$ ) or even excellent agreement (Azimuth:  $ICC = 0.92$ ). It seems that, in absence of structural abnormalities, the plane for both reference axes is very similar, suggesting that both reference systems could be used interchangeable for tilt measurements. In the present study it was observed that the IOL power might have a slight influence on IOL decentration after implantation. Nonetheless, this effect was different depending on the reference system selected. It was significant for the X-coordinate using the iridocorneal angle

system and for the Y-coordinate using the pupil center system. Therefore, these outcomes emphasize the importance of selecting a proper reference system based on the primary outcome measure targeted, because both reference systems are not interchangeable.

The mean internal and ocular HOAs found after uneventful implantation of the Tecnis ZCB00 are in concordance with Song et al. [24], who used same IOL and pupil diameter. For a 4 mm pupil diameter, we found that the mean ocular primary SA was  $-0.018 \mu\text{m}$ , and  $-0.064 \mu\text{m}$  the internal one (Table 1). The



**Table 3.** Coordinates with a significant effect on ocular HOAs.

Ocular HOAs	Reference system	Coordinate	$\beta$ (95% CI)	P-value
$Z_3^{-3}$	Pupil	Y	-0.25 (-0.50/0.01)	0.057
$Z_3^1$	Pupil	Y	0.13 (0.05/0.22)	0.004
$Z_4^{-4}$	Pupil	X	0.08 (0.01/0.15)	0.028
$Z_3^3$	Iridocorneal angles	X	-0.27 (-0.47/-0.07)	0.010
$Z_4^2$	Iridocorneal angles	Y	0.08 (0.04/0.13)	0.001
$Z_4^2$	Iridocorneal angles	Polar angle	$-0.01 \times 10^{-3}$ ( $-0.02 \times 10^{-3}/-0.01 \times 10^{-3}$ )	0.004
Primary coma (RMS)	Iridocorneal angles	X	-0.10 (-0.19/-0.02)	0.019
Primary coma (RMS)	Iridocorneal angles	Y	-0.09 (-0.14/-0.04)	0.001
Coma-like (RMS)	Iridocorneal angles	X	-0.10 (-0.19/-0.02)	0.019
Coma-like (RMS)	Iridocorneal angles	Y	-0.09 (-0.14/-0.04)	0.002

CI confidence interval, HOAs higher-order aberrations, RMS root mean square.

aspheric design of the IOL compensated the corneal SA resulting in a mean ocular SA value close to zero, while the mean internal SA was similar to the value reported for the Tecnis ZCB00 IOL at 4 mm ( $-0.05 \mu\text{m}$ ) [25].

The lack of significant results in the present study for the second-order Zernike coefficients suggests that the ZCB00 decentration and tilt found has no important impact on the postoperative refraction. In addition, the influence of IOL decentration on internal and ocular oblique trefoil ( $Z_3^3$ ) was significant for X-coordinate using the iridocorneal angles system. It was observed that the longer the temporal displacement was, the higher the internal and ocular aberrations were. Fernández-Sánchez et al. [26], showed that low values of induced coma and trefoil (0.13 and 0.17  $\mu\text{m}$ , respectively) had no effect on VA or contrast sensitivity. Considering the regression coefficients of our results for  $Z_3^3$  ( $\beta = -0.19$  and  $\beta = -0.27$  internal and ocular, respectively), it would require higher decentration values, approximately 0.62 mm, to induce a  $Z_3^3$  value of at least 0.17  $\mu\text{m}$ . Therefore, our results suggest that the level of IOL decentration after uneventful surgery is not high enough to negatively affect postoperative quality of vision from a clinical viewpoint.

We did not find any other influence of IOL decentration on internal HOAs except for the abovementioned internal and ocular oblique trefoil ( $Z_3^3$ ). However, we found that the IOL decentration, using the pupil center as reference system, had an effect on three ocular HOAs: vertical trefoil ( $Z_3^{-3}$ ), horizontal coma ( $Z_3^1$ ) and vertical tetrafoil ( $Z_4^{-4}$ ). And using the iridocorneal angles system, IOL decentration had an effect on ocular primary coma, coma-like and vertical secondary astigmatism ( $Z_4^2$ ). The fact that these results were only found in ocular HOAs but not in internal ones, could suggest that the IOL has minimal or no influence. Nevertheless, the magnitude of the relationships found ( $-0.25 \leq \beta \leq 0.13$ ) appears to be too low to be considered as clinically relevant.

Tecnis ZCB00 tilt did not have a significant effect on VA or internal and ocular HOAs. Similarly, previous authors [27] (only abstract available in English) reported that the tilt of Tecnis ZCB00 had no significant effect on internal HOAs. Therefore, IOL tilt appears not to have a clinically relevant impact on visual quality, when tilt values are representative of the ones commonly observed after uneventful Tecnis ZCB00 implantations.

Some authors have described tolerable decentration and tilt values after the implantation of aspheric IOLs. Holladay et al. [7], reported that an aspherical IOL allows a better wavefront quality than a spherical one even under a decentration <0.4 mm and tilt <7 degrees. Likewise, Piers et al. [28] observed better optical quality in aspherical IOLs decentered <0.8 mm and tilted <10 degrees, in comparison with spherical ones. However, decentration and tilt values simulated at experimental settings could be

higher than values observed in the clinical practice [29, 30], as occurs in our study sample. Thus, the influence of aspheric pseudophakic IOL decentration and tilt observed in clinical practice appears to have negligible effects on the quality of vision.

One limitation of the present study could be that a pupil diameter of 4 mm was selected for HOAs analyses. This diameter was used because it is close to the one usually found in population older than 70 years in mesopic conditions [31]. Additionally, it must be considered that smaller pupil diameters could considerably decrease the magnitude of the HOAs measured, while larger diameters could not represent our sample. Finally, a large effect size was considered to estimate sample size, expecting to achieve the most relevant findings. However, most of the significant results found in the present study were considered to have low clinical impact. Thus, future studies selecting smaller effect sizes are likely to find outcomes of even lower clinical relevance.

In conclusion, the IOL decentration and tilt values commonly observed after in-the-bag implantation of the aspheric pseudophakic Tecnis ZCB00, considering the pupil and iridocorneal angles as reference systems, result in ocular and internal HOAs that are not high enough to negatively affect quality of vision from a clinically relevant viewpoint. Additionally, pupil and iridocorneal angles considered as reference systems can be used interchangeably for IOL tilt measurements when assessed with ss-OCT technology. In contrast, IOL decentration measures are different depending on the reference system considered.

## Summary

What was known before

- Tecnis ZCB00 has an aspheric design inducing a negative spherical aberration of  $-0.27 \mu\text{m}$  with the aim of compensating the spherical aberration of the cornea.
- Decentration and tilt of aspheric intraocular lenses could unbalance higher order aberrations and visual acuity having a negative impact on optical quality.

What this study adds

- Tecnis ZCB00 decentration and tilt values commonly observed after uneventful implantations result in visual acuity and higher order aberrations that appear not to have a clinical impact on quality of vision.
- Pupil and iridocorneal angles used as reference systems could be interchangeable for pseudophakic intraocular lens tilt measurements, but not for decentration ones.

- It is described a new technique to assess decentration and tilt of pseudophakic intraocular lens based on swept-source optical coherence tomography images that provides high reliable estimations.

## DATA AVAILABILITY

The datasets generated during and/or analyzed during the current study are available from the corresponding author on reasonable request.

## REFERENCES

- Smith G, Cox MJ, Calver R, Garner LF. The spherical aberration of the crystalline lens of the human eye. *Vis Res.* 2021;41:235–43.
- Amano S, Amano Y, Yamagami S, Miyai T, Miyata K, Samejima T, et al. Age-related changes in corneal and ocular higher-order wavefront aberrations. *Am J Ophthalmol.* 2004;137:988–92.
- Alió JL, Schimchak P, Negri HP, Montés-Micó R. Crystalline lens optical dysfunction through aging. *Ophthalmology.* 2005;112:2022–9.
- Davis G. The evolution of cataract surgery. *Mo Med.* 2016;113:58–62.
- Barbero S, Marcos S, Jiménez-Alfaro I. Optical aberrations of intraocular lenses measured in vivo and in vitro. *J Opt Soc Am A Opt Image Sci Vis.* 2003;20:1841–51.
- Montés-Micó R, Ferrer-Blasco T, Cerviño A. Analysis of the possible benefits of aspheric intraocular lenses: review of the literature. *J Cataract Refract Surg.* 2009;35:172–81.
- Holladay JT, Piers PA, Koranyi G, van der Mooren M, Norrby NES. A new intraocular lens design to reduce spherical aberration of pseudophakic eyes. *J Refract Surg.* 2002;18:683–91.
- Schrecker J, Langenbucher A, Seitz B, Eppig T. First results with a new intraocular lens design for the individual correction of spherical aberration. *J Cataract Refract Surg.* 2018;44:1211–9.
- Schrecker J, Schröder S, Langenbucher A, Seitz B, Eppig T. Individually customized IOL versus standard spherical aberration-correcting IOL. *J Refract Surg.* 2019;35:565–74.
- Mester U, Dillinger P, Anterist N. Impact of a modified optic design on visual function: clinical comparative study. *J Cataract Refract Surg.* 2003;29:652–60.
- Bellucci R, Scialdone A, Buratto L, Morselli S, Chiarego C, Crisculi A, et al. Visual acuity and contrast sensitivity comparison between Tecnis and AcrySof SA60AT intraocular lenses: a multicenter randomized study. *J Cataract Refract Surg.* 2005;31:712–7.
- Trueb PR, Albach C, Montés-Micó R, Ferrer-Blasco T. Visual acuity and contrast sensitivity in eyes implanted with aspheric and spherical intraocular lenses. *Ophthalmology.* 2009;116:890–5.
- Morales EL, Rocha KM, Chalita MR, Nosé W, Avila MP. Comparison of optical aberrations and contrast sensitivity between aspheric and spherical intraocular lenses. *J Refract Surg.* 2011;27:723–8.
- Schuster AK, Tesarz J, Vossmerbaeumer U. The impact on vision of aspheric to spherical monofocal intraocular lenses in cataract surgery: a systematic review with meta-analysis. *Ophthalmology.* 2013;120:2166–75.
- Pérez-Gracia J, Varea A, Ares J, Vallés JA, Remón L. Evaluation of the optical performance for aspheric intraocular lenses in relation with tilt and decenter errors. *PLoS One.* 2020;15:e0232546.
- Mamalis N, Brubaker J, Davis D, Espandar L, Werner L. Complications of foldable intraocular lenses requiring explantation or secondary intervention—2007 survey update. *J Cataract Refract Surg.* 2008;34:1584–91.
- Fujikado T, Saika M. Evaluation of actual retinal images produced by misaligned aspheric intraocular lenses in a model eye. *Clin Ophthalmol.* 2014;8:2415–23.
- Pérez-Merino P, Marcos S. Effect of intraocular lens decentration on image quality tested in a custom model eye. *J Cataract Refract Surg.* 2018;44:889–96.
- Lawu T, Mukai K, Matsushima H, Senoo T. Effects of decentration and tilt on the optical performance of 6 aspheric intraocular lens designs in a model eye. *J Cataract Refract Surg.* 2019;45:662–8.
- Ashena Z, Maqsood S, Ahmed SN, Nanavaty MA. Effect of intraocular lens tilt and decentration on visual acuity, dysphotopsia and wavefront aberrations. *Vision.* 2020;14:41.
- Cohen J. *Statistical power analysis of the behavioural sciences.* 2nd ed. New York: Academic Press; 1988.
- Koo TK, Li MY. A guideline of selecting and reporting intraclass correlation coefficients for reliability research. *J Chiropr Med.* 2016;15:155–63.
- Song WK, Lee JA, Kim JY, Kim MJ, Tchah H. Analysis of positional relationships of various centers in cataract surgery. *Korean J Ophthalmol.* 2019;33:70–81.
- Song IS, Kim MJ, Yoon SY, Kim JY, Tchah H. Higher-order aberrations associated with better near visual acuity in eyes with aspheric monofocal IOLs. *J Refract Surg.* 2014;30:442–6.
- Petermeier K, Frank C, Gekeler F, Spitzer MS, Messias A, Szurman P. Influence of the pupil size on visual quality and spherical aberration after implantation of the Tecnis 1-piece intraocular lens. *Br J Ophthalmol.* 2011;95:42–45.
- Fernández-Sánchez V, Ponce ME, Lara F, Montés-Micó R, Castejón-Mochón JF, López-Gil N. Effect of 3rd-order aberrations on human vision. *J Cataract Refract Surg.* 2008;34:1339–44.
- Yu F, Chang P, Li J, Zhou Y, Zhao Y. Comparative study of the tilt, decentration and higher-order aberrations (HOA) of single-piece and 3-piece Tecnis aspheric intraocular lenses. *Zhonghua Yan Ke Za Zhi.* 2015;51:270–5.
- Piers PA, Weeber HA, Artal P, Norrby S. Theoretical comparison of aberration-correcting customized and aspheric intraocular lenses. *J Refract Surg.* 2007;23:374–84.
- Baumeister M, Bühren J, Kohlen T. Tilt and decentration of spherical and aspheric intraocular lenses: effect on higher-order aberrations. *J Cataract Refract Surg.* 2009;35:1006–12.
- Miyata K, Kataoka Y, Matsunaga J, Honbo M, Minami K. Prospective comparison of one-piece and three-piece Tecnis aspheric intraocular lenses: 1-year stability and its effect on visual function. *Curr Eye Res.* 2015;40:930–5.
- Tekin K, Sekeroglu MA, Kiziltoprak H, Doguiz S, Inanc M, Yilmazbas P. Static and dynamic pupillometry data of healthy individuals. *Clin Exp Optom.* 2018;101:659–65.

## AUTHOR CONTRIBUTIONS

Concept and design: EP, NEH, PJB. Acquisition, analysis, or interpretation of data: All authors. Methodological development and statistical analysis: EMP, EP, AJAC, ALR. Drafting of the paper: EMP, ALR, ALM, MJM. Critical revision of the paper for important intellectual content: All authors.

## FUNDING

EM-P was supported by Junta de Castilla y León and European Social Fund (EDU/1100/2017). The funders of the study had no role in study design, data collection, data analysis, data interpretation, or writing of the report.

## COMPETING INTERESTS

PJB reports grants from Bausch and Lomb, Zeiss and Medcontur outside the scope of the submitted work. The rest of the authors declare no competing interests.

## ADDITIONAL INFORMATION

**Supplementary information** The online version contains supplementary material available at <https://doi.org/10.1038/s41433-022-02211-2>.

**Correspondence** and requests for materials should be addressed to Alberto López-Miguel.

**Reprints and permission information** is available at <http://www.nature.com/reprints>

**Publisher's note** Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.

Springer Nature or its licensor holds exclusive rights to this article under a publishing agreement with the author(s) or other rightsholder(s); author self-archiving of the accepted manuscript version of this article is solely governed by the terms of such publishing agreement and applicable law.