

RESEARCH

Open Access



Refractive outcomes of table-mounted and hand-held auto-refractometers in children: an observational cross-sectional study

Müjdat Karabulut*, Sinem Karabulut and Aylin Karalezli

This is to certify that: The article has not been presented in a meeting. The authors did not receive any financial support from any public or private sources. The authors have no financial or proprietary interest in a product, method, or material described herein.

Abstract

Background: To compare the refractive results of hand-held and table-mounted autorefractors.

Methods: We designed this study as an observational, cross-sectional study. We compared the mean spherical and cylinder power, spherical equivalent, Jackson cross-cylinder values, determined the limits of agreement (LoA), and evaluated the reliability of two autorefractors.

Results: We evaluated 256 eyes of 256 pediatric patients (mean age, 9.12 ± 2.26 years; range, 5–16 years). 49% of the patients were female, and 51% were male. The Nidek HandyRef-K autorefractor measured relatively more astigmatism ($P < 0.001$) and less hyperopia ($P = 0.024$). The mean differences and 95% LoA were $0.06 \text{ D} \pm 0.47 \text{ D}$ (-0.82 D to 0.98 D) in spherical power, $0.08 \text{ D} \pm 0.28 \text{ D}$ (-0.47 D to 0.64 D) in cylindrical power, $0.11 \text{ D} \pm 0.47 \text{ D}$ (-0.81 D to 1.01 D) in spherical equivalent, $0.02 \text{ D} \pm 0.36 \text{ D}$ (-0.73 D to 0.69 D) in Jackson cross-cylinder power at 0° , $0.005 \text{ D} \pm 0.54 \text{ D}$ (-1.07 D to 1.06 D) in Jackson cross-cylinder power at 45° . We found the difference within 0.50 D in 244 (95%) eyes for spherical power, in 245 (96%) eyes for cylindrical power, 228 (89%) eyes for spherical equivalent, 224 (87%) eyes for Jackson cross-cylinder power at 0° , 213 (83%) eyes for Jackson cross-cylinder power at 45° . When comparing devices, there were strong correlations for spherical power (Spearman's $\rho = 0.99$, $P < 0.001$), cylindrical power (Spearman's $\rho = 0.88$, $P < 0.001$), and spherical equivalent (Spearman's $\rho = 0.98$, $P < 0.001$).

Conclusion: Two autorefractors showed clinically applicable agreement limits; excellent reliability for spherical power and spherical equivalent and good reliability for cylindrical power; high positive percent agreement for spherical and cylindrical power, spherical equivalent, Jackson cross-cylinder power at 0° and 45° . These results showed that both devices might be used interchangeably for screening of refractive error in children.

Keywords: Autorefractors, Cylindrical power, Jackson cross-cylinder, Spherical equivalent spherical power

Introduction

Amblyopia is a unilateral or, rarely, bilateral reduction of best-corrected visual acuity that cannot be attributed directly to the effect of any structural abnormality of the eye or visual pathways [1]. It is also a neurodevelopmental disorder associated with the visual cortex and lateral

*Correspondence: mujdatkarabulut@gmail.com
Department of Ophthalmology, Mugla Sıtkı Koçman University Medical School, 48300 Mugla, Turkey



© The Author(s) 2021. **Open Access** This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>. The Creative Commons Public Domain Dedication waiver (<http://creativecommons.org/publicdomain/zero/1.0/>) applies to the data made available in this article, unless otherwise stated in a credit line to the data.

geniculate nucleus abnormalities [2, 3]. Refractive amblyopia is a type of amblyopia and consists of ametropic, meridional, and anisometropic subtypes [4]. Ametropic amblyopia may arise from bilateral 5.0–6.0 Diopter (D) or more myopia and 4.0–5.0 D or more hyperopia. Meridional amblyopia may happen in the presence of 2.0–3.0 D or more astigmatism. Anisometropic amblyopia may arise from anisomyopia (3.0–4.0 D or more), anisoastigmatism (2.0 D or more), and anisohyperopia (1.0–1.5 D or more) [5]. Therefore, timely identification of refractive errors in children is crucial for preventing refractive amblyopia. For this purpose, national pediatric vision screening programs have been planned and may vary among countries depending on the country's income [6]. Cycloplegic retinoscopy is the gold standard for evaluating refractive errors in children because refractive error can be obtained objectively by completely relaxing accommodation with this method [7, 8]. However, it is time-consuming and requires an experienced clinician.

The autorefractors have an essential role in preventing the development of refractive amblyopia by accurately screening the amblyogenic refractive errors. Various techniques, such as hand-held and table-mounted autorefractometers, are commonly used to detect refractive errors [9]. Although these devices rapidly measure the refractive errors and provide valid results, they are bulky, non-portable, and not appropriate for immobile patients [10].

On the other hand, hand-held auto-refractometers are small, portable, and can be used anywhere as needed. They are also practical and appropriate for newborns, infants, and bedridden patients or those with reduced mobility restricting their sitting ability.

Reliability determines the consistency or correlation of two values measured with different people or the same person at different times [11]. If the two devices give reliable results, they can be used interchangeably.

In this cross-sectional study, we compared the cycloplegic measurements of a table-mounted (Topcon TRK-2P; Topcon Medical Systems, Inc., Tokyo, Japan) and hand-held (Nidek HandyRef-K; Nidek Co., Ltd., Tokyo, Japan) auto-refractometer, and determined the limits of agreement (LoA) and reliability of both devices.

Methods

Pediatric patients who visited the ophthalmology clinic for regular ocular examination were enrolled in this observational cross-sectional study. We included the children, aged 5 to 16 years, who have no history of ocular surgery (Corneal, lenticular, or retinal surgery), sensitivity to cyclopentolate, epilepsy, and were able to cooperate enough with the measurements to gather reliable results. We excluded those patients with manifest strabismus

or motility disorders; nystagmus; media opacity; congenital or acquired corneal, lenticular, retinal, choroidal, or optic disc abnormalities; and participants who were unable to cooperate with the measurements. After informing the patients and their parents or legal representatives, the authors obtained consent from children, parents, or legal representatives. All patients underwent comprehensive ocular examination, including visual acuity, anteroposterior segments check, ocular motility, and the cover-uncover test. Cyclopentolate 1% (Cycloplegin; Abdi Ibrahim, Istanbul, Turkey) was applied three times at intervals of 5 min. Patients waited for about 45 min to attain complete cycloplegia and dilated pupils that did not react to intense light. The evaluations were performed randomly in the same room and light condition, with the Topcon TRK-2P and Nidek HandyRef-K devices operated by a single expert blinded to the study. This expert was a trained professional with 9 years of experience in a clinical setting and did not know the participants' personal information and study's name, purpose, and design until the study was over.

Measurement accuracy check was performed daily with a 0.12 D model eye for both devices before the evaluations. Since the measured results (0.12 D) did not differ from the values indicated on the model eye, the devices were not calibrated. Additionally, the same devices were used throughout the study.

The Nidek HandyRef-K is a closed-field hand-held, portable, easy-to-use, monocular auto-refractometer that detects refractive errors in infants, any age of childhood, and adolescents sitting, standing, or in a supine position. A fogging mechanism is exerted to reduce accommodation. Its measurement range is -20.00 D to $+20.00$ D sphere (0.12 D/0.25 D increments), cylinder 0 D to 12.00 D (0.12 D/0.25 D increments), and axis 0° to 180° ($1^\circ/5^\circ$ increments) [12].

Topcon TRK-2P is a table-mounted instrument that assembles a refractor keratometer, non-contact tonometer, and pachymeter in one device. However, these devices are large, difficult to move, and not appropriate for bedridden patients, infants, or any patient who cannot sit down to have measurements taken. The refractive measurement range of Topcon TRK-2P is -30 D to $+25$ D sphere (0.12 D/0.25 D increments), 0 D to 12 D cylinder (0.12 D/0.25 D increments), and 0° to 180° ($1^\circ/5^\circ$ increments) astigmatic axis [13]. Topcon TRK-2P also uses a fogging mechanism to diminish accommodation.

The standard refractometer model was used for both devices. We averaged three consecutive, valid cycloplegic measurements of spherical power (S_{pwr}), cylindrical power (C_{pwr}), and cylindrical axis (C_{ax}) for each device. We analyzed average values in the Statistical Package for the Social Sciences (SPSS) version 21.0.0.0. If three

consecutive measurements from each device differed by more than 0.50 D, repeated evaluations were done until the variations decreased below 0.50 D to get valid results.

The spherical equivalent (SE) and Jackson cross-cylinder power at 0° (J_0) and 45° (J_{45}) axis were computed using the following formulas: $SE = S_{pwr} + C_{pwr}/2$; $J_0 = -(C_{pwr}/2) \cos 2C_{ax}$; and $J_{45} = -(C_{pwr}/2) \sin 2C_{ax}$, respectively. Because the refractive errors of two eyes are correlated, measurements of the left eyes were analyzed.

All subjects were divided into subgroups according to the mean S_{pwr} and C_{pwr} of the Topcon TRK-2P values. The subgroups were designed considering the American Academy of Ophthalmology guidelines for correcting more than -3.00 D and $+4.50$ D isoametropia, -3.00 D and $+1.50$ D anisometropia, 2.00 D astigmatic refractive error in young children to prevent the development of refractive amblyopia [5]. This guideline was used only for classification into subgroups. Although our participants' age ranged from 5 to 16 years, we wanted to compare the measurement of the two devices and define the differences in these amblyogenic refractive errors. We also compared the mean astigmatic refractive error under 1.00 D since it is mostly seen in clinical practice.

The positive percent agreement (PPA) is a proportion of individuals with the target condition by the imperfect reference standard who test positive. It can be used to determine the accuracy of two devices in the absence of the gold standard [14]. We calculated PPA within 0.5 D by estimating the proportion of difference within 0.5 D for all parameters.

After testing the normality and homogeneity of variables with the Shapiro-Wilk, Kolmogorov-Smirnov and Levene's tests ($p < 0.05$ for all variables with all tests), the Wilcoxon signed-rank test was performed. The Bland-Altman plot was generated to determine the 95% LoA. Spearman's rank correlation coefficient was used to assess reliability. Spearman's rank correlation coefficient equal to or greater than 0.9 and between 0.8 and 0.9 demonstrated excellent and good reliability. $P < 0.05$ was respected as statistically significant.

Results

Two hundred seventy patients were enrolled, and 14 of them were excluded from the study due to exclusion criteria (Eight invalid results, five manifest strabismus, one choroidal coloboma). The left eyes of 256 Caucasian pediatric patients were evaluated in this study. The gender distribution was 127 females (49%) and 129 males (51%). Sixty-nine (26.9%) of the patients had a type of refractive amblyopia (29 [11.3%] ametropic, 26 [10.2%] anisometropic, 14 [5.5%] meridional amblyopia) when they enrolled in the study. The mean age (\pm standard

deviation [SD]) was 9.12 ± 2.26 years (range, 5–16 years). Figure 1 shows the age distribution.

When comparing the two devices, there were no significant differences in S_{pwr} , J_0 , or J_{45} ($P = 0.191$, $P = 0.560$, $P = 0.247$, respectively) (Table 1). However, compared to Topcon TRK-2P, the Nidek HandyRef-K autorefractor measured more astigmatism (mean C_{pwr} , $P < 0.001$), less hyperopia (SE, $P = 0.024$) regarding the mean SE, and significantly bigger C_{ax} ($P = 0.037$) (Table 1).

The mean differences and 95% LoA were: for S_{pwr} , $0.06 \text{ D} \pm 0.47 \text{ D}$ (-0.82 D to 0.98 D) (Fig. 2); for C_{pwr} , $0.08 \text{ D} \pm 0.28 \text{ D}$ (-0.47 D to 0.64 D) (Fig. 3); for SE, $0.11 \text{ D} \pm 0.47 \text{ D}$ (-0.81 D to 1.01 D) (Fig. 4); for J_0 , $0.02 \text{ D} \pm 0.36 \text{ D}$ (-0.73 D to 0.69 D) (Fig. 5); and for J_{45} , $0.005 \text{ D} \pm 0.54 \text{ D}$ (-1.07 D to 1.06 D) (Fig. 6). We found the difference within 0.50 D in 244 (95%) eyes for S_{pwr} , in 245 (96%) eyes for C_{pwr} , 228 (89%) eyes for SE, 224 (87%) eyes for J_0 , 213 (83%) eyes for J_{45} .

When comparing the two devices, there was a strong correlation for S_{pwr} (Spearman's $\rho = 0.99$, $P < 0.001$), C_{pwr} (Spearman's $\rho = 0.88$, $P < 0.001$), SE (Spearman's $\rho = 0.98$, $P < 0.001$); a moderate positive correlation for J_0 (Spearman's $\rho = 0.32$, $P < .001$); and a weak positive correlation for J_{45} (Spearman's $\rho = 0.17$, $P = 0.018$) (Table 2).

In our subgroup analyses, compared to the Topcon TRK-2P, the Nidek HandyRef-K device showed significantly less hyperopia in two subgroups: those with S_{pwr} values between $+1.50$ D and $+4.50$ D and those with S_{pwr} values more than $+4.50$ D ($P = 0.031$ and 0.045 , respectively). Also, compared to the Topcon TRK-2P, the Nidek HandyRef-K device showed more myopia in the myopia subgroup with S_{pwr} values of more than -3.00 D ($P = 0.026$, Table 3).

Compared to the Topcon TRK-2P, in the subgroup with C_{pwr} less than -1.00 D, the Nidek HandyRef-K device also detected more C_{pwr} and significantly different C_{ax} values ($P < 0.001$, $P = 0.025$, respectively; Table 4).

Discussion

Our findings showed that in the early detection of amblyogenic refractive errors, two auto-refractometers might be used interchangeably in children who were capable of adequate cooperation during measurement. Additionally, in children who have poor collaboration during measurement, the Nidek HandyRef-K could be used instead of Topcon TRK-2P. In the subgroup analysis, the differences between the measurements of the two auto-refractometers were likely to be within clinically applicable limits though there were some minor differences.

Some studies have been reported the reliability and agreement limits of auto-refractometers. For example, Ying GS et al. [15] evaluated the agreement limit

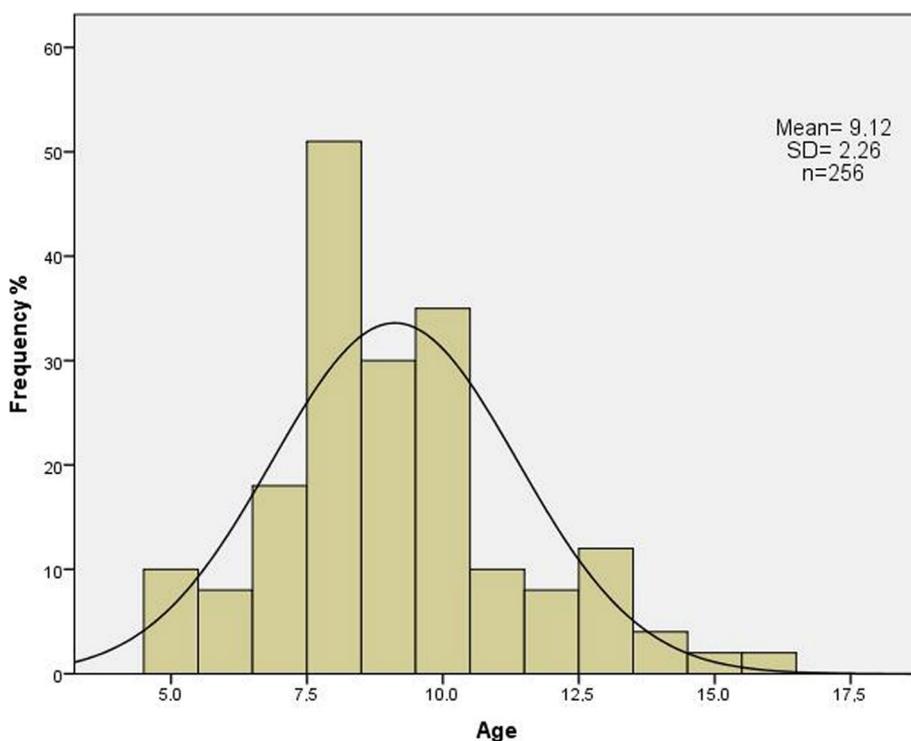


Fig. 1 The age (years) distribution of the enrolled patients (n = 256)

Table 1 Comparison of the refractive measurement of two devices in all eyes

	Topcon TRK-2P	Nidek Handy Ref-K	P-value
S_{pwr} (D) Mean \pm SD	2.23 \pm 3.45	2.17 \pm 3.39	0.191
Range	(-4.50)- (15.25)	(-4.75)- (14.75)	
C_{pwr} (D) Mean \pm SD	-0.75 \pm 0.83	-0.84 \pm 0.85	<0.001
Range	(-4.75)- (0.00)	(-5.00)- (0.00)	
C_{ax} (°) Mean \pm SD	82.84 \pm 72.94	100.38 \pm 74.42	0.037
Range	0-180	0-180	
SE (D) Mean \pm SD	1.85 \pm 3.35	1.75 \pm 3.30	0.024
Range	(-4.88)- (14.88)	(-5.25)- (14.50)	
J_0 (D) Mean \pm SD	-0.08 \pm 0.36	-0.06 \pm 0.36	0.560
Range	(-1.99)- (1.80)	(-1.57)- (1.90)	
J_{45} (D) Mean \pm SD	-0.05 \pm 0.42	-0.04 \pm 0.47	0.247
Range	(-2.16)- (1.54)	(-1.92)- (2.40)	

S_{pwr} Spherical power, C_{pwr} Cylindrical power, C_{ax} Cylindrical axes, SE Spherical equivalent, SD Standard deviation, D Diopter, J_0 Jackson cross-cylinder power at 0° axis, J_{45} Jackson cross-cylinder power at 45° axis

of a table-mounted and hand-held auto-refractometer and reported that mean differences and 95% LoA were 0.34 D (-0.46 D to 1.14 D) for S_{pwr} ; 0.18 D (-0.47 D to 0.64 D) for C_{pwr} ; 0.25 D (-0.55 D to 1.05 D) for SE. They reported the proportion of differences within the accuracy of 0.50 D as 56.9% for S_{pwr} and 70.2% for SE.

Additionally, Büchner TF et al. [16] reported the proportion of differences within the accuracy of 0.50 D as 18.2% for SE, 82.1 for C_{pwr} , and 66.6 for C_{ax} .

Sayed KM et al. [17] compared table-mounted and hand-held auto-refractometer measurements and found strong positive correlations for S_{pwr} and C_{pwr} . The hand-held auto-refractometer measured more myopia regarding SE. They reported good agreement limits for C_{pwr} despite the relatively poor agreement limits for SE, J_0 , and J_{45} . Iuorno JD et al. [18] also reported that a hand-held auto-refractometer measured more myopia than a table-mounted auto-refractometer regarding SE though it had reliable results for C_{pwr} .

The accuracy of auto-refractometers' measurements of S_{pwr} , C_{pwr} , SE, and C_{ax} , varies depending on cycloplegia. Mirzajani et al. [19] reported prominent variation in the S_{pwr} , SE, and J_{45} vector between a table-mounted and a hand-held auto refractometer in non-cycloplegic condition. These authors found a strong positive correlation and fair agreement for S_{pwr} , SE, J_0 , and J_{45} vectors.

Akil et al. [10] compared outcomes of hand-held and table-mounted auto-refractometer. They evaluated significantly hyperopic results for mean SE with the table-mounted auto-refractometer before cycloplegia. Good agreement and no significant differences were obtained

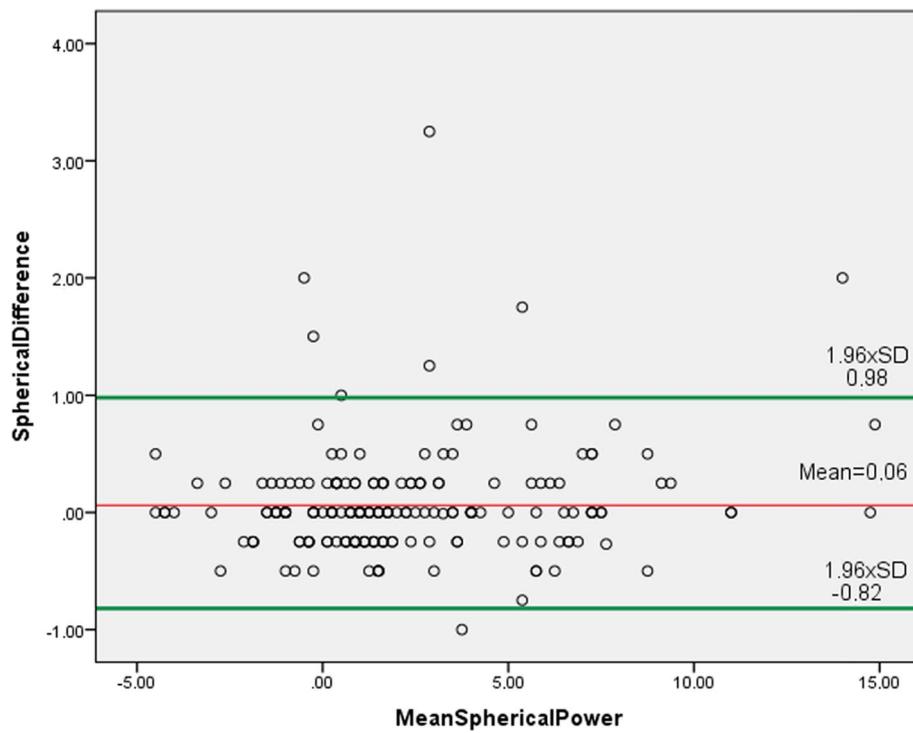


Fig. 2 Bland Altman plot showing the agreement between Topcon TRK-2P and Nidek HandyRef-K for the mean spherical power. The middle line demonstrates the mean difference of spherical power (0.06 D \pm 0.47 D), and the other two side lines show the 95% limits of agreement (-0.82 D to 0.98 D)

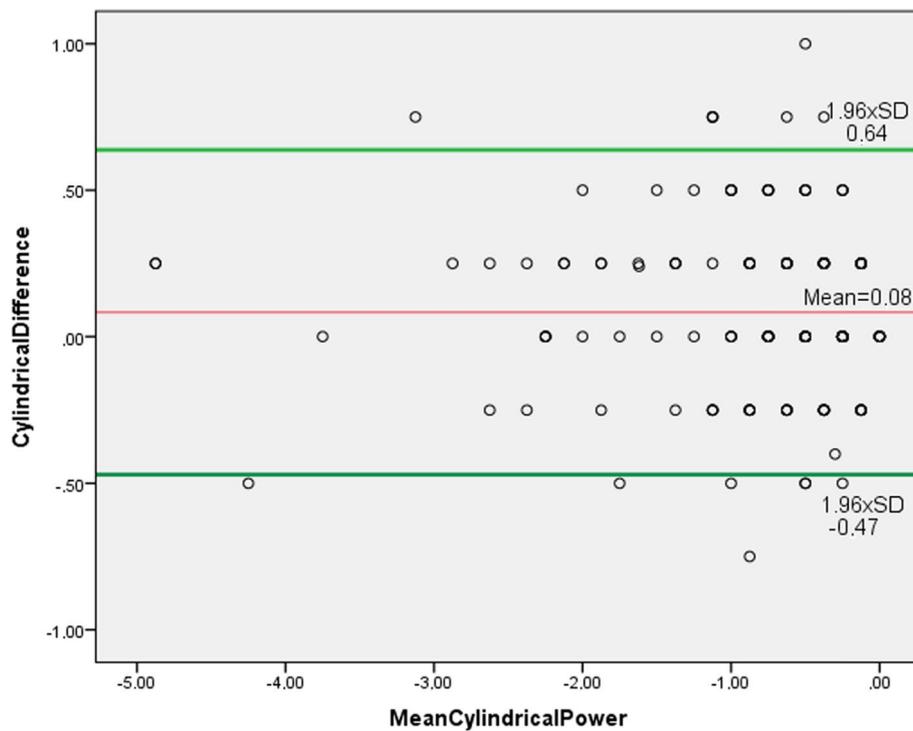


Fig. 3 Bland Altman plot showing the agreement between Topcon TRK-2P and Nidek HandyRef-K for the mean cylindrical power. The middle line demonstrates the mean difference (0.08 D \pm 0.28 D), and the other two side lines show the 95% limits of agreement (-0.47 D to 0.64 D)

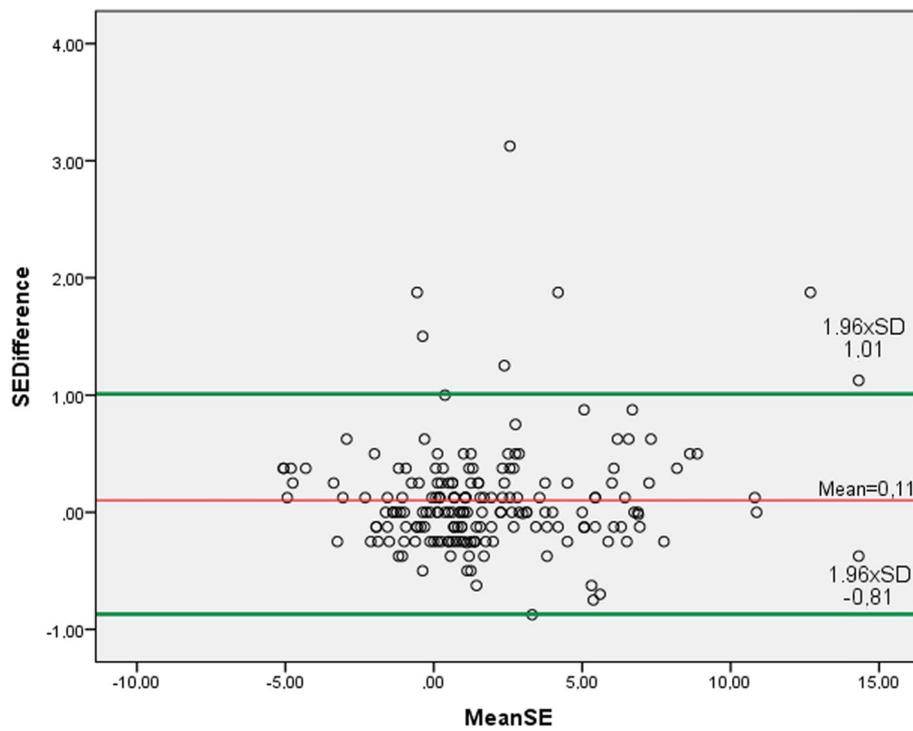


Fig. 4 Bland Altman plot showing the agreement between Topcon TRK-2P and Nidek HandyRef-K for the mean spherical equivalent. The middle line demonstrates the mean difference (0.11 D ± 0.47 D), and the other two side lines show the 95% limits of agreement (− 0.81 D to 1.01 D)

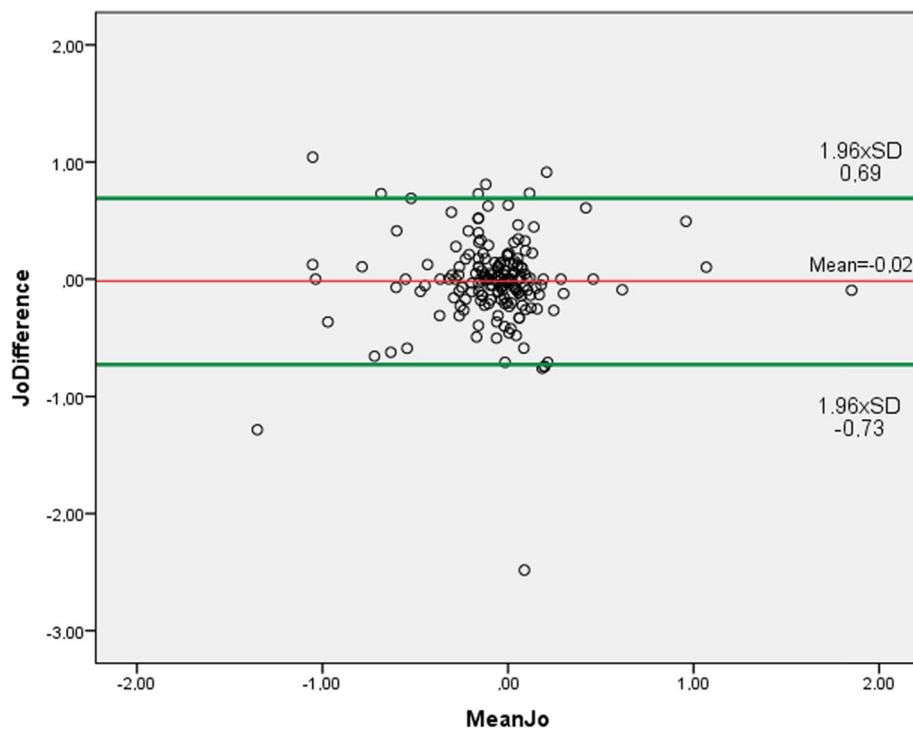


Fig. 5 Bland Altman plot showing the agreement between Topcon TRK-2P and Nidek HandyRef-K for the mean Jackson cross-cylinder power at 0°. The middle line demonstrates the mean difference (0.02 D ± 0.36 D), and the other two side lines show the 95% limits of agreement (− 0.73 D to 0.69 D)

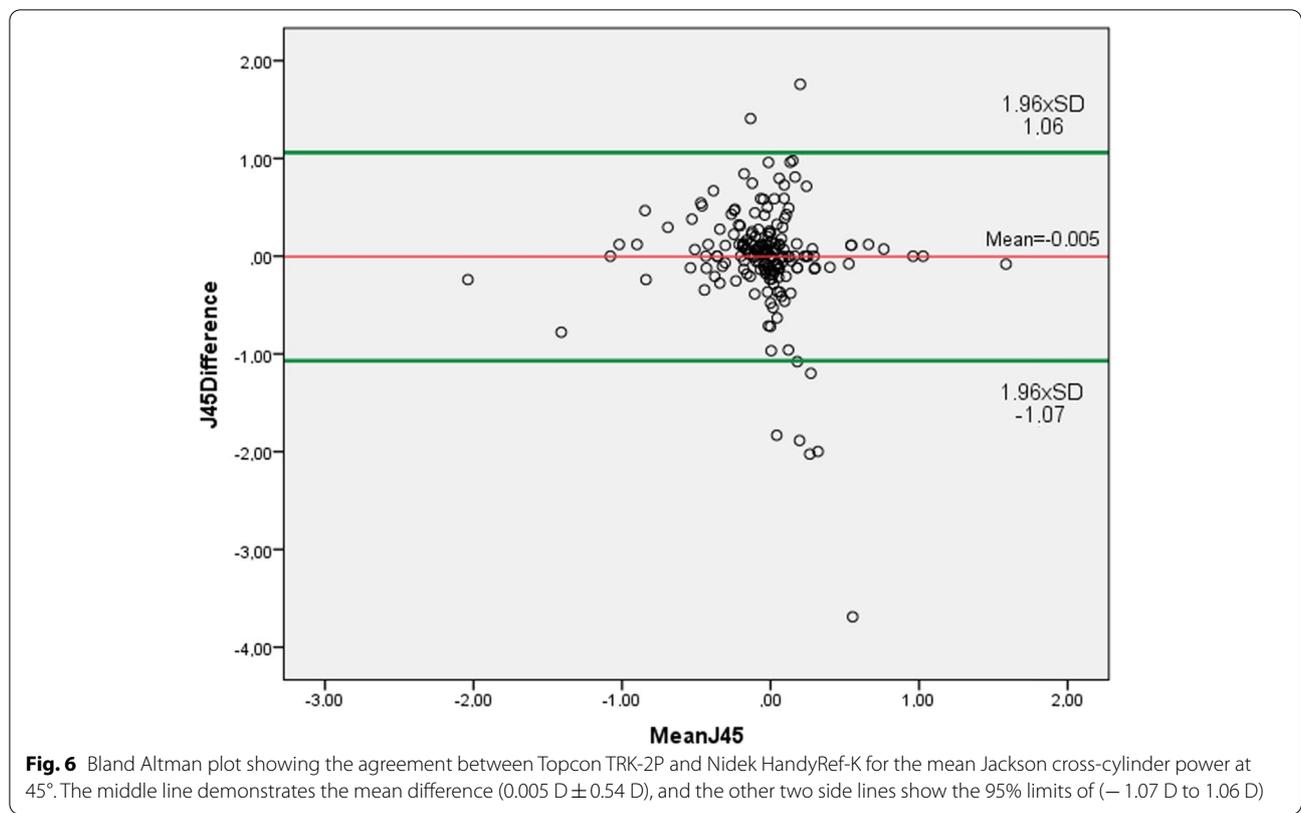


Table 2 The reliability of two devices for S_{pwr} , C_{pwr} , SE, J_0 , and J_{45} with Spearman's correlation coefficient

	S_{pwr}	C_{pwr}	SE	J_0	J_{45}
Rho	0.99	0.88	0.98	0.32	0.17
p-value	<0.001	<0.001	<0.001	<0.001	0.018

S_{pwr} Spherical power, C_{pwr} Cylindrical power, SE Spherical equivalent, J_0 Jackson cross-cylinder power at 0° axis, J_{45} Jackson cross-cylinder power at 45° axis, Rho Spearman's rho

for S_{pwr} , C_{pwr} , J_0 , and J_{45} among two devices and cycloplegic retinoscopy after cycloplegia.

In a cross-sectional study, Oral et al. [20] evaluated the cycloplegic results of a hand-held autorefractor with

cycloplegic retinoscopy and reported no significant difference in terms of mean S_{pwr} , C_{pwr} , and SE, and a strong correlation among devices.

Farook et al. [21] compared a hand-held autorefractor with a table-mounted autorefractor and subjective refraction. They found that the hand-held autorefractor measured more myopia than the table-mounted autorefractor and subjective refraction. However, their measurements were in non-cycloplegic condition and included only adult participants.

Seymen et al. [22] compared three hand-held autorefractors (HandyRef-K, Retinomax, and Plusoptix). These authors reported no significant difference among the three hand-held devices for the mean S_{pwr} and C_{ax} .

Table 3 Comparison of the mean S_{pwr} of two devices in the subgroups for S_{pwr}

Subgroup for S_{pwr}	Age (Year) Mean (Range)	N	Topcon TRK-2P Mean ± SD	Nidek Handy Ref-K	P-value
$S_{pwr} \geq -3.00D$	11.11(6–14)	24	−4.19 ± 0.77	−4.40 ± 0.90	0.026
$0.00D \leq S_{pwr} < -3.00D$	7.98(5–15)	76	−1.14 ± 0.45	−1.18 ± 0.38	0.541
$0.00 \leq S_{pwr} < +1.50D$	8.22 (5–16)	54	0.62 ± 0.53	0.58 ± 0.78	0.305
$+1.50D \leq S_{pwr} < +4.50D$	7 (5–13)	61	2.01 ± 1.02	1.87 ± 1.06	0.031
$S_{pwr} \geq +4.50D$	6.12 (5–13)	41	6.75 ± 2.64	6.51 ± 2.61	0.045

S_{pwr} Spherical power, SD Standard deviation, D Diopter, N Number

Table 4 Comparison of the mean C_{pwr} , axis, and Jackson cross-cylinder power in the subgroups for C_{pwr}

Subgroup for C_{pwr}	Age (Year) Mean (Range)	N	Topcon TRK-2P Mean \pm SD	Nidek Handy Ref-K	P-value
$C_{pwr} \geq -2.00$	6.2 (5–13)	64			
C_{pwr} (D)			-2.42 ± 0.95	-2.49 ± 0.97	0.245
C_{ax} ($^{\circ}$)			106.11 ± 79	130.37 ± 68.52	0.262
J_0 (D)			-0.26 ± 0.86	-0.21 ± 0.80	0.831
J_{45} (D)			-0.26 ± 0.93	0.03 ± 1.1	0.447
$-1.00D \leq C_{pwr} < -2.00$	6.5 (5–14)	51			
C_{pwr} (D)			-1.13 ± 0.13	-1.05 ± 0.34	0.355
C_{ax} ($^{\circ}$)			76.19 ± 76.71	78.1 ± 79.51	0.134
J_0 (D)			-0.12 ± 0.30	-0.18 ± 0.38	0.709
J_{45} (D)			0.03 ± 0.48	-0.12 ± 0.36	0.351
$C_{pwr} < -1.00D$	7.9 (5–16)	141			
C_{pwr} (D)			-0.38 ± 0.25	-0.52 ± 0.34	< 0.001
C_{ax} ($^{\circ}$)			79.22 ± 71.11	97.71 ± 73.74	0.025
J_0 (D)			-0.04 ± 0.15	-0.02 ± 0.18	0.251
J_{45} (D)			-0.02 ± 0.17	-0.05 ± 0.24	0.171

C_{pwr} Cylindrical power, C_{ax} Cylindrical axes, SD Standard deviation, D Diopter, J_0 Jackson cross-cylinder power at 0° axis, J_{45} Jackson cross-cylinder power at 45° axis

However, the mean SE measured with Plusoptix was significantly more myopic compared to those measured with the HandyRef-K and Retinomax devices. The authors also found that the mean C_{pwr} measured by the HandyRef-K device was considerably higher compared to Plusoptix and Retinomax. In their study, refractive measurements with the Plusoptix device were taken in non-cycloplegic conditions, while those with HandyRef-K and Retinomax were in cycloplegic states. Moreover, these authors did not compare the mean J_0 and J_{45} values.

Astigmatism is a significant amblyogenic factor. Yap et al. [23] showed that lower magnitudes of astigmatism could also cause amblyopia and meridional deficits in the visual cortex of the newly diagnosed meridional amblyopic patients. Some studies reported that prevalences of meridional amblyopia were 30, 35, and 63% in patients with high astigmatism [24, 25]. This current study showed that meridional amblyopia was present in only 14 (21.9%) of the 64 patients who had 2.0 D or more astigmatism. This relatively lower percentage may be related to the fact that most patients were not newly diagnosed and had been complying well with spectacles and patching treatment that prevented them from getting amblyopia. This study had some limitations. The primary flaw was not comparing the results with cycloplegic retinoscopy. Unfortunately, we could not measure cycloplegic retinoscopy from all patients due to technical problems with the device when the study continued and did not gather enough cycloplegic retinoscopy results for the comparison. We only compared the measurements of two devices with each other, not

with the results of cycloplegic retinoscopy. Therefore this study could not determine which device was more accurate. We also did not compare the repeatability of S_{pwr} , C_{pwr} , and C_{ax} with either device.

In conclusion, the two autorefractors showed clinically applicable agreement limits, high PPA within 0.50 D for S_{pwr} , C_{pwr} , SE, J_0 , and J_{45} , excellent reliability for S_{pwr} and SE, and good reliability for C_{pwr} in cycloplegic conditions, though the Nidek HandyRef-K measured more astigmatism and less hyperopia in comparing the mean C_{pwr} and SE, and there existed some minor differences in subgroup analysis. The results from this current study showed that both devices might be used interchangeably for making clinical decisions and pediatric refractive screening. These differences, agreement intervals, and reliability of two auto-refractometers should be kept in mind in clinical practice and national pediatric vision screening programs to correct the refractive error.

Acknowledgments

Not applicable.

Significance

Here, we compare the results using two auto-refractometers (the Topcon TRK-2P and Nidek HandyRef) among pediatric patients. Compared to Topcon TRK-2P, the Nidek HandyRef-K auto-refractometer measured significantly less hyperopia regarding the mean spherical equivalent and more astigmatism. In addition, the Nidek HandyRef-K device detected less hyperopia and more myopia in comparing the mean spherical power within subgroups. Two devices showed high PPA within 0.50 D for S_{pwr} , C_{pwr} , SE, J_0 , and J_{45} . Both devices showed excellent reliability for S_{pwr} and SE, good reliability for C_{pwr} , and clinically applicable agreement limits for all measurements. They may be used interchangeably for making clinical decisions and pediatric refractive error screening.

Authors' contributions

Müjdat Karabulut, Sinem Karabulut, and Aylin Karalezli have made substantial contributions to conception and design, data acquisition, analysis, and data interpretation. Müjdat Karabulut, Sinem Karabulut, and Aylin Karalezli have given final approval of the version to be published. All the authors agree to be accountable for all aspects of the work in ensuring that questions related to the accuracy or integrity of any part of the work are appropriately investigated and resolved.

Funding

This research did not take any specific grant from funding agencies in the public, commercial, or not-for-profit sectors.

Availability of data and materials

All data generated or analyzed during this study are included in this published article.

Declarations**Ethics approval and consent to participate**

In this study's procedures, we followed the local institutional research committee's ethical standards and the 1964 Helsinki declaration of ethical standards. Informed consent was gathered from all individual participants and their parents. Muğla Sıtkı Koçman University Clinical Research Ethics Committee arranged ethical approval.

Consent for publication

Not applicable.

Competing interests

The authors have no financial or proprietary interest in a product, method, or material described herein.

Received: 16 January 2021 Accepted: 1 December 2021

Published online: 09 December 2021

References

- Amblyopia. In: Robert WH, Steven MA, Rebecca SB, Arif OK, Katherine AL, Gregg TL, Mary AO, Kristina TH. editors. 2019–2020 BCSC (Basic and Clinical Science Course), Section 06: Pediatric Ophthalmology and Strabismus. San Francisco: American Academy of Ophthalmology; 2019. p. 79–86.
- Mortazavi M, Aigner KM, Antono JE, Gambacorta C, Nahum M, Levi DM, et al. Neural correlates of visual spatial selective attention are altered at early and late processing stages in human amblyopia. *Eur J Neurosci*. 2021;53(4):1086–106.
- Barnes GR, Li X, Thompson B, Singh KD, Dumoulin SO, Hess RF. Decreased gray matter concentration in the lateral geniculate nuclei in human amblyopes. *Invest Ophthalmol Vis Sci*. 2010;51(3):1432–8.
- Wallace DK, Chandler DL, Beck RW, Arnold RW, Bacal DA, Birch EE, et al. Treatment of bilateral refractive amblyopia in children three to less than 10 years of age. *Am J Ophthalmol*. 2007;144(4):487–96.
- Types of Amblyopia. <https://www.aaio.org/disease-review/types-of-amblyopia>. 21 Oct 2015.
- Chen AH, Abu Bakar NF, Arthur P. Comparison of the pediatric vision screening program in 18 countries across five continents. *J Curr Ophthalmol*. 2019;31(4):357–65.
- Schimitzek T, Haase W. Efficiency of a video-auto refractometer used as a screening device for amblyogenic factors. *Graefes Arch Clin Exp Ophthalmol*. 2002;240(9):710–6.
- Jorge J, Queirós A, Almeida JB, Parafita MA. Retinoscopy/autorefractometry: which is the best starting point for a noncycloplegic refraction? *Optom Vis Sci*. 2005;82(1):64–8.
- Group PEDIG. The clinical profile of moderate amblyopia in children younger than seven years. *Arch Ophthalmol*. 2002;120(3):281–7.
- Akil H, Keskin S, Çavdarlı C. Comparison of the refractive measurements with a hand-held auto refractometer, table-mounted auto refractometer, and cycloplegic retinoscopy in children. *Korean J Ophthalmol*. 2015;29(3):178–84.
- Lachin JM. The role of measurement reliability in clinical trials. *Clin Trials*. 2004;1(6):553–66.
- Handheld Ref/Keratometer / Handheld Refractometer. <http://dfv.com.au/resources/product-brochures/diagnostic/Nidek-HandyRef-K-HandyRef.pdf>. 2015.
- TRK-2P, Kerato-refractometer, Tono-pachymeter. <https://www.topcon-medical.eu/eu/products/294-trk-2p-kerato-refractometer-tono-pachymeter.html#downloads>. 2018.
- Biswas B. Clinical performance evaluation of molecular diagnostic tests. *J Mol Diagn*. 2016;18(6):803–12.
- Ying GS, Maguire MG, Kulp MT, Ciner E, Moore B, Pistilli M, et al. Comparison of cycloplegic refraction between grand Seiko autorefractor and Retinomax autorefractor in the vision in preschoolers-hyperopia in preschoolers (VIP-HIP) study. *J AAPOS*. 2017;21(3):219–223.e3.
- Büchner TF, Schnorbus U, Grenzebach UH, Stupp T, Busse H. Examination of preschool children for refractive errors. First experience using a hand-held autorefractor. *Ophthalmologie*. 2003;100(11):971–8.
- Sayed KM, Alsmman AH, Mostafa EM. Hand-held Nidek versus table-mounted Huvitz autorefractors and their agreement with subjective refraction in adults. *Clin Ophthalmol*. 2021;15:1391–401.
- luorno JD, Grant WD, Noel LP. Clinical comparison of the Welch Allyn SureSight hand-held autorefractor versus cycloplegic autorefractometry and retinoscopic refraction. *J AAPOS*. 2004;8(2):123–7.
- Mirzajani A, Qasemi F, Asharilous A, Yekta A, Doostdar A, Khabazkhoob M, et al. Are the results of hand-held auto-refractometer as valid as the result of table-mounted refractometer? *J Curr Ophthalmol*. 2018;31(3):305–11.
- Oral Y, Gunaydin N, Ozgur O, Arsan A, Oskan S. A comparison of different autorefractors with retinoscopy in children. *J Pediatr Ophthalmol Strabismus*. 2012;49(6):370–7.
- Farook M, Venkatramani J, Gazzard G, Cheng A, Tan D, Saw SM. Comparisons of the hand-held autorefractor, table-mounted autorefractor, and subjective refraction in Singapore adults. *Optom Vis Sci*. 2005;82(12):1066–70.
- Seymen Z, Vural E, Eris E, Vural A, Ogreden T, Aslan O, et al. Comparison of the latest hand-held auto refracto-keratometer with Retinomax and Plusoptix in patients younger than three years of age. *Beyoglu Eye J*. 2019;4:32–7.
- Yap TP, Luu CD, Suttle C, Chia A, Boon MY. Effect of stimulus orientation on visual function in children with refractive amblyopia. *Invest Ophthalmol Vis Sci*. 2020;61(5):5.
- Harvey EM, Dobson V, Miller JM. Prevalence of high astigmatism, eyeglass wear, and poor visual acuity among native American grade school children. *Optom Vis Sci*. 2006;83(4):206–12.
- Dobson V, Miller JM, Harvey EM, Mohan KM. Amblyopia in astigmatic preschool children. *Vis Res*. 2003;43(9):1081–90.

Publisher's Note

Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.

Ready to submit your research? Choose BMC and benefit from:

- fast, convenient online submission
- thorough peer review by experienced researchers in your field
- rapid publication on acceptance
- support for research data, including large and complex data types
- gold Open Access which fosters wider collaboration and increased citations
- maximum visibility for your research: over 100M website views per year

At BMC, research is always in progress.

Learn more biomedcentral.com/submissions

