

ERRATUM

Erratum to: Intraoperative Tumor Detection Using a Ratiometric Activatable Fluorescent Peptide: A First-in-Human Phase 1 Study

Jonathan T. Unkart, MD, MS¹, Steven L. Chen, MD, MBA², Irene L. Wapnir, MD³, Jesús E. González, PhD², Alec Harootunian, PhD², and Anne M. Wallace, MD¹

¹Department of Surgery, Moores Cancer Center, University of California, San Diego, La Jolla, CA; ²Avelas Biosciences, Inc., La Jolla, CA; ³Department of Surgery, Stanford University, Stanford, CA

ERRATUM TO: ANN SURG ONCOL DOI 10.1245/S10434-017-5991-3

In the original article there is an error in Fig. 3. Following is the corrected Fig. 3.

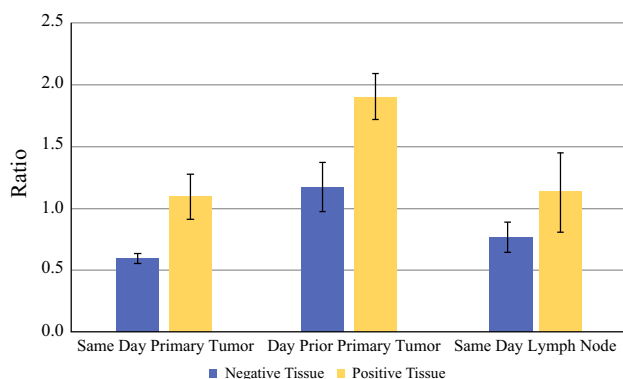


FIG. 3 Tissue ratio of malignant versus negative tissue. Average Cy5/Cy7 ratio measurements from region of interest (ROI) versus non-malignant adjacent tissue are shown. The *error bars* represent standard deviations

The online version of the original article can be found under doi:[10.1245/s10434-017-5991-3](https://doi.org/10.1245/s10434-017-5991-3).

© Society of Surgical Oncology 2017

Published Online: 31 July 2017

A. M. Wallace, MD
e-mail: amwallace@ucsd.edu